
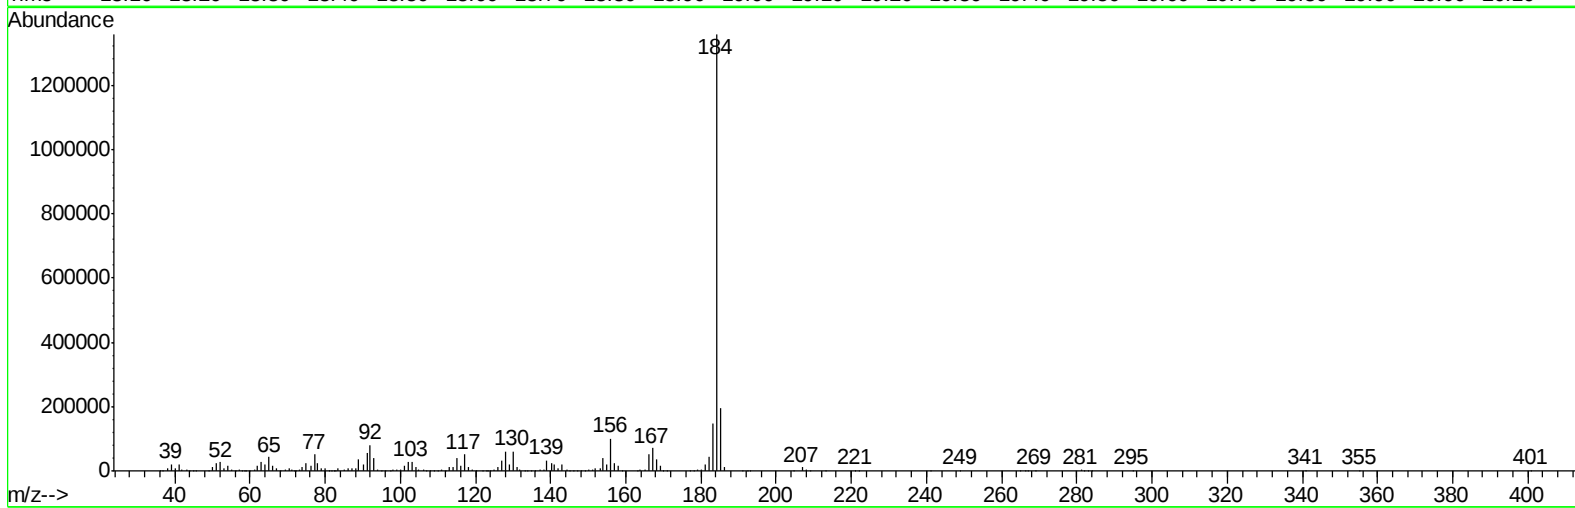


Data Path : Z:\HPCHEM1\BNA M\DATA\BM071817\
Data File : BM010876.D
Acq On : 18 Jul 2017 18:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 06:24:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

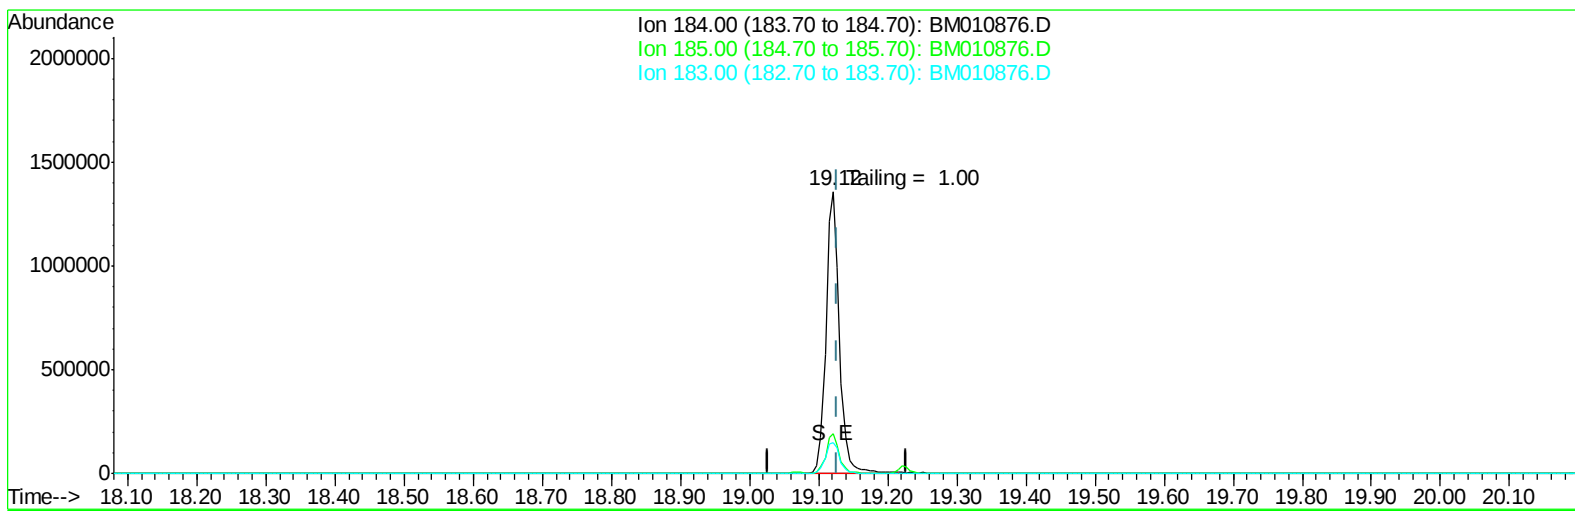

TIC: BM010876.D

(76) Benzidine



19.121min (-0.006) 19998.54ng

response 1817956

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.31
183.00	11.10	10.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071817\
Data File : BM010876.D
Acq On : 18 Jul 2017 18:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 06:24:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

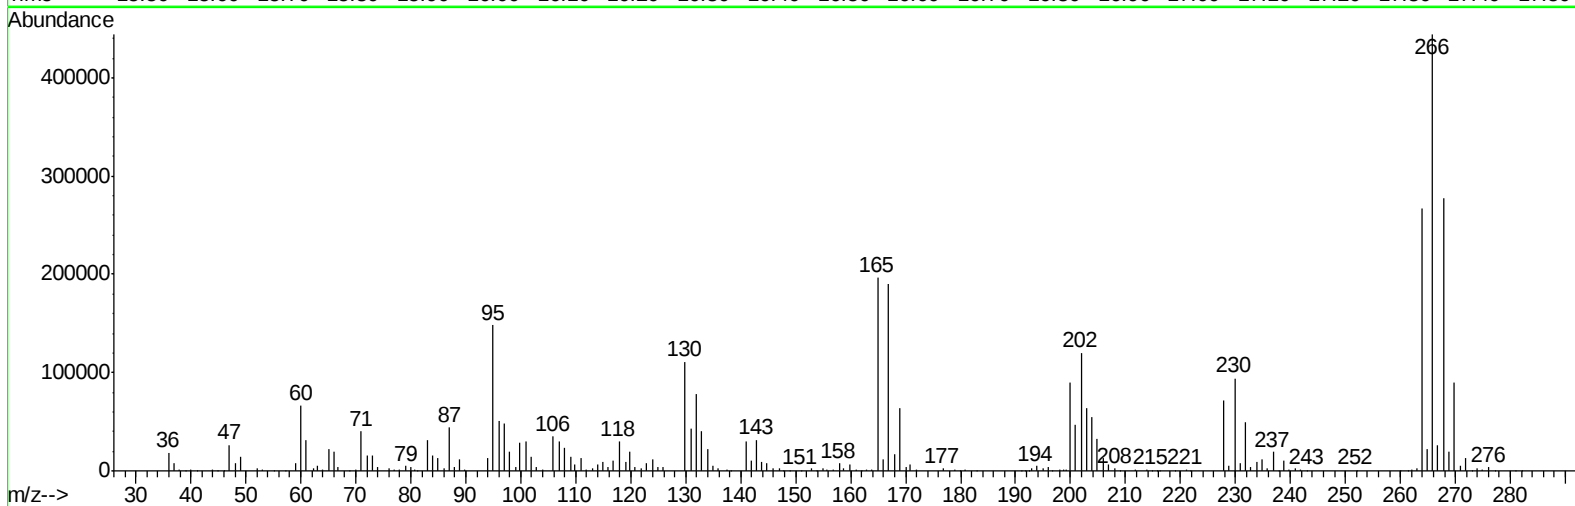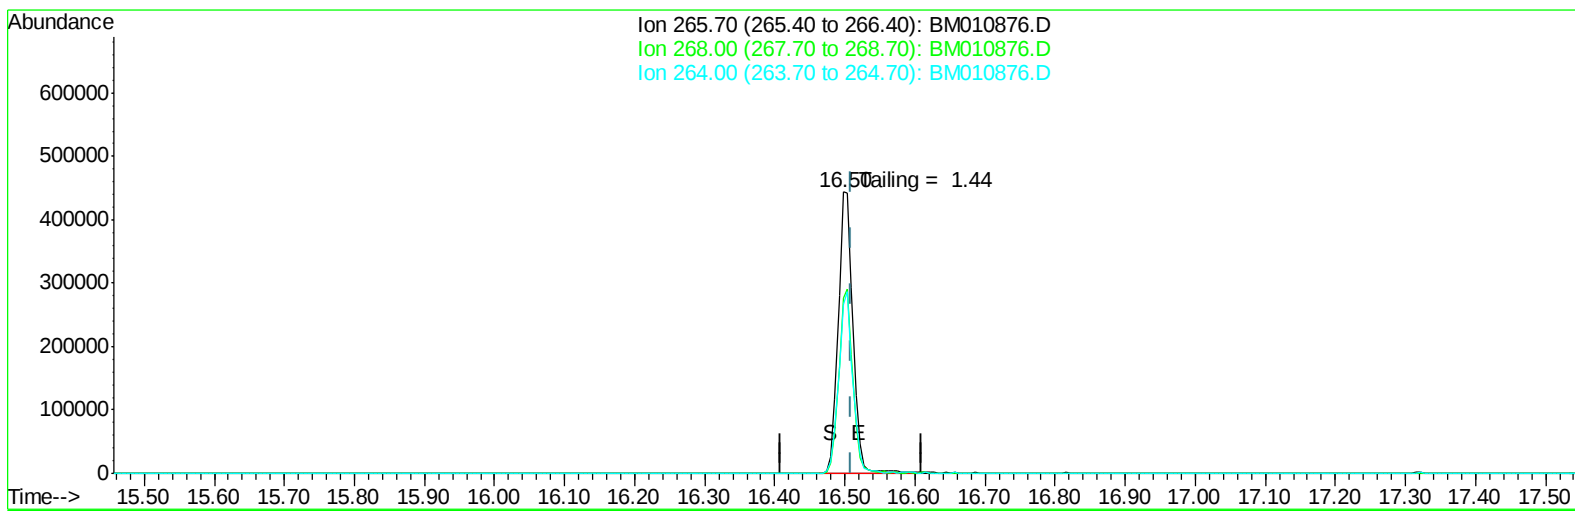

TIC: BM010876.D

(69) Pentachlorophenol (C)

16.498min (-0.012) 44100.40ng

response 637071

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.44
264.00	61.20	60.10
0.00	0.00	0.00