


Data Path : Z:\HPCHEM1\BNA M\DATA\BM071817\
 Data File : BM010876.D
 Acq On : 18 Jul 2017 18:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

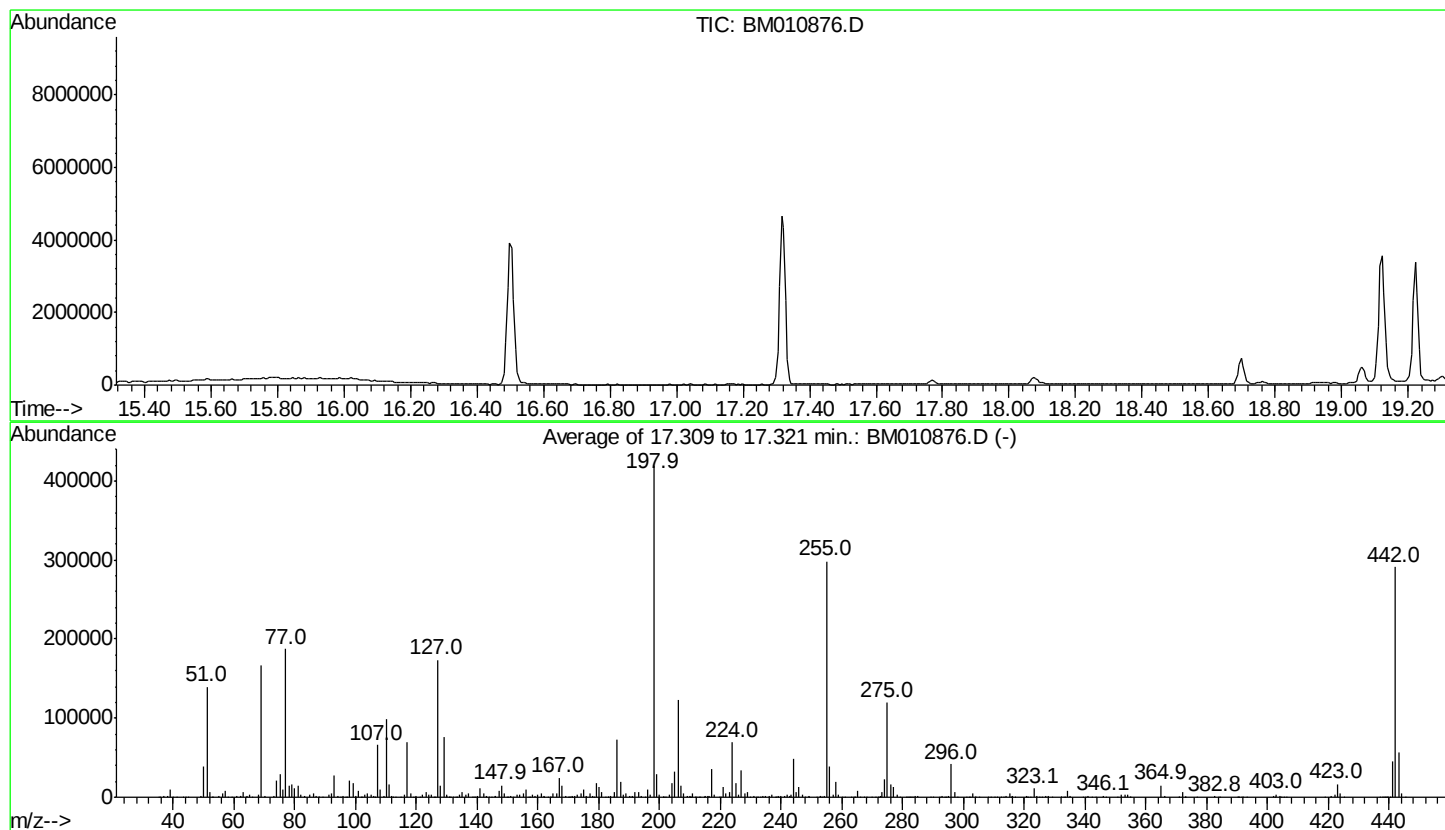

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	139568	PASS
68	69	0.00	2	1.7	2877	PASS
69	198	0.00	100	39.6	166037	PASS
70	69	0.00	2	0.7	1108	PASS
127	198	10	80	41.4	173653	PASS
197	198	0.00	2	0.6	2665	PASS
198	198	100	100	100.0	419242	PASS
199	198	5	9	6.8	28688	PASS
275	198	10	60	28.5	119554	PASS
365	198	1	100	3.6	14977	PASS
441	443	0.01	100	78.1	44808	PASS
442	198	50	100	69.5	291221	PASS
443	442	15	24	19.7	57341	PASS