


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071822\
 Data File : BM035849.D
 Acq On : 18 Jul 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 18 17:08:15 2022

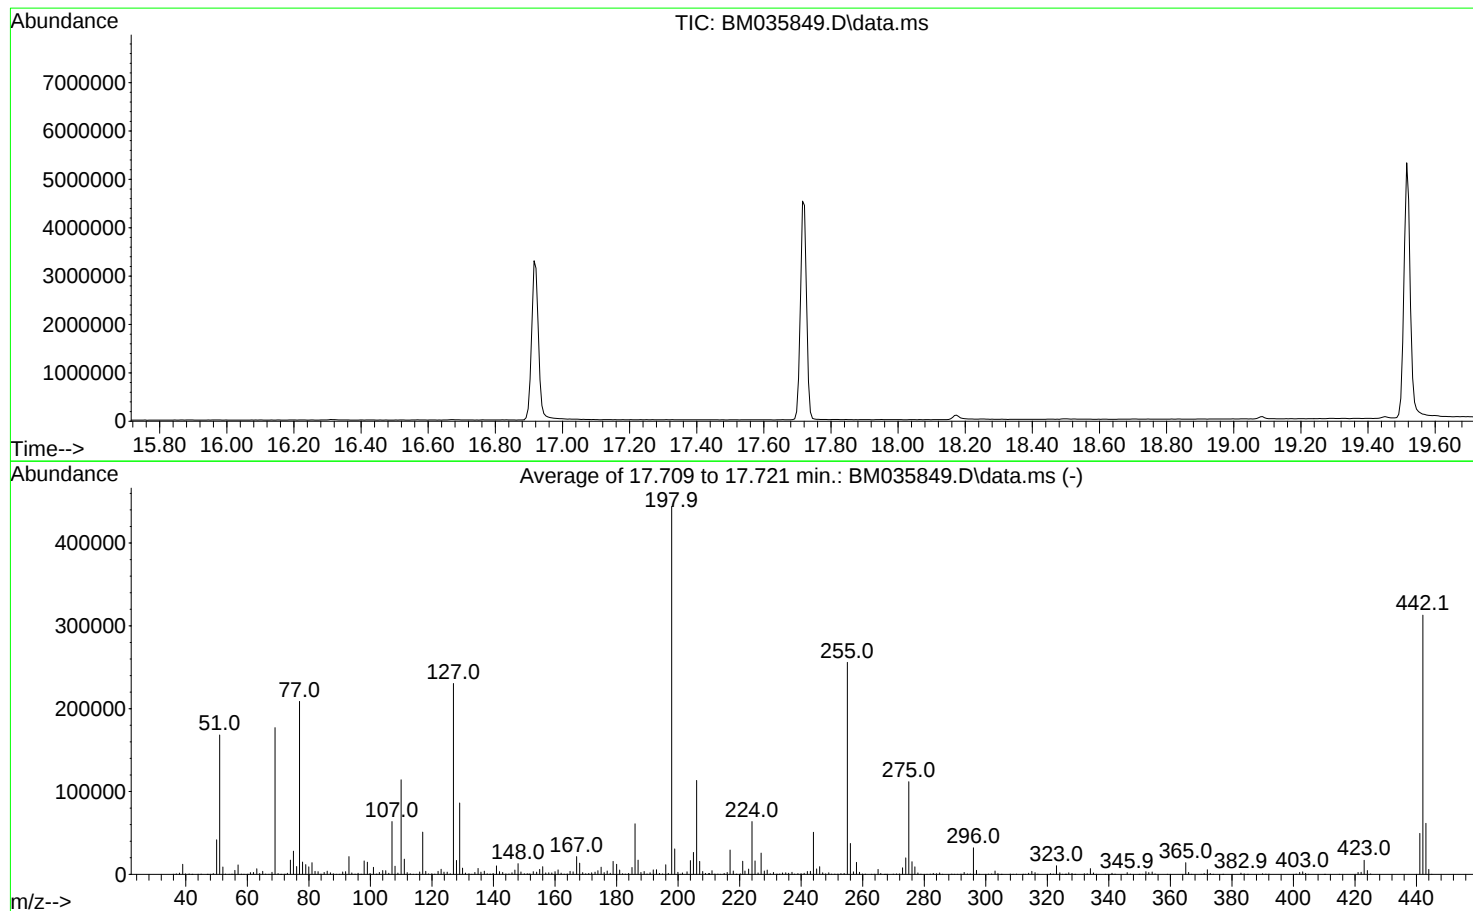




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	168293	PASS
68	69	0.00	2	1.4	2483	PASS
69	198	0.00	100	39.9	177169	PASS
70	69	0.00	2	0.5	927	PASS
127	198	10	80	51.9	230528	PASS
197	198	0.00	2	0.3	1162	PASS
198	198	100	100	100.0	444117	PASS
199	198	5	9	6.9	30627	PASS
275	198	10	60	25.2	111899	PASS
365	198	1	100	3.2	14052	PASS
441	198	0.01	100	11.2	49531	PASS
442	442	50	100	100.0	313003	PASS
443	442	15	24	19.7	61651	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071822\
Data File : BM035849.D
Acq On : 18 Jul 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 18 15:03:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 18 14:58:17 2022
Response via : Initial Calibration

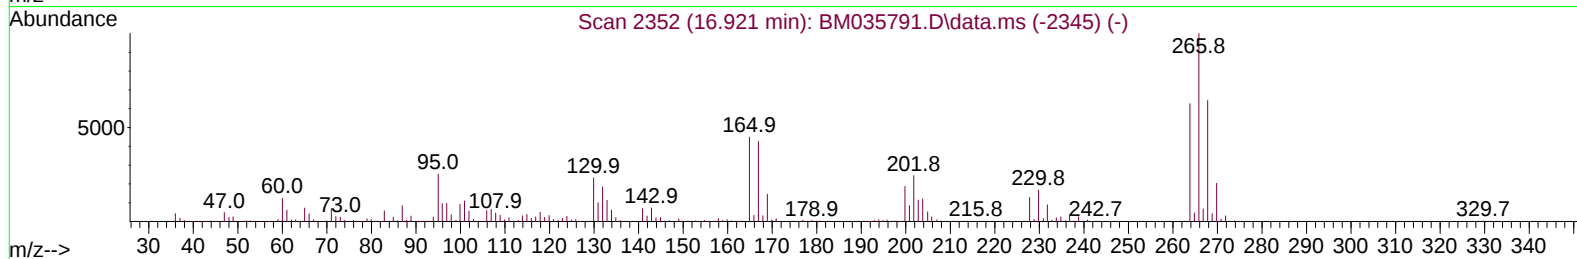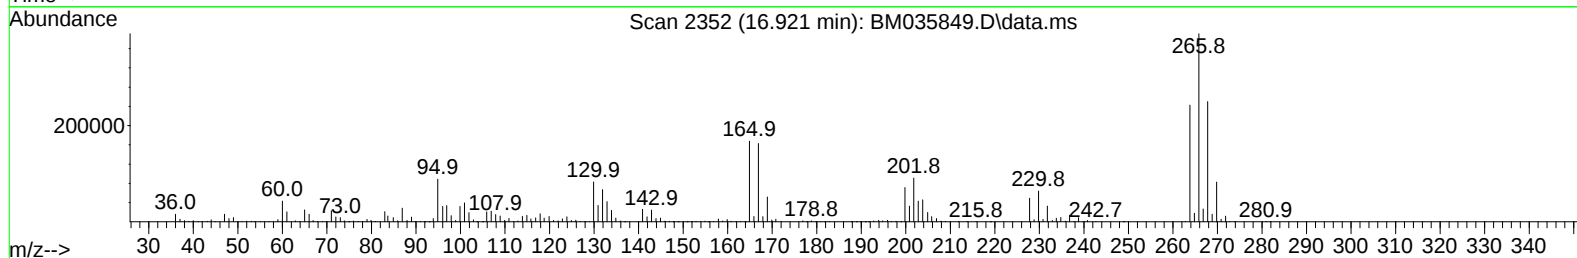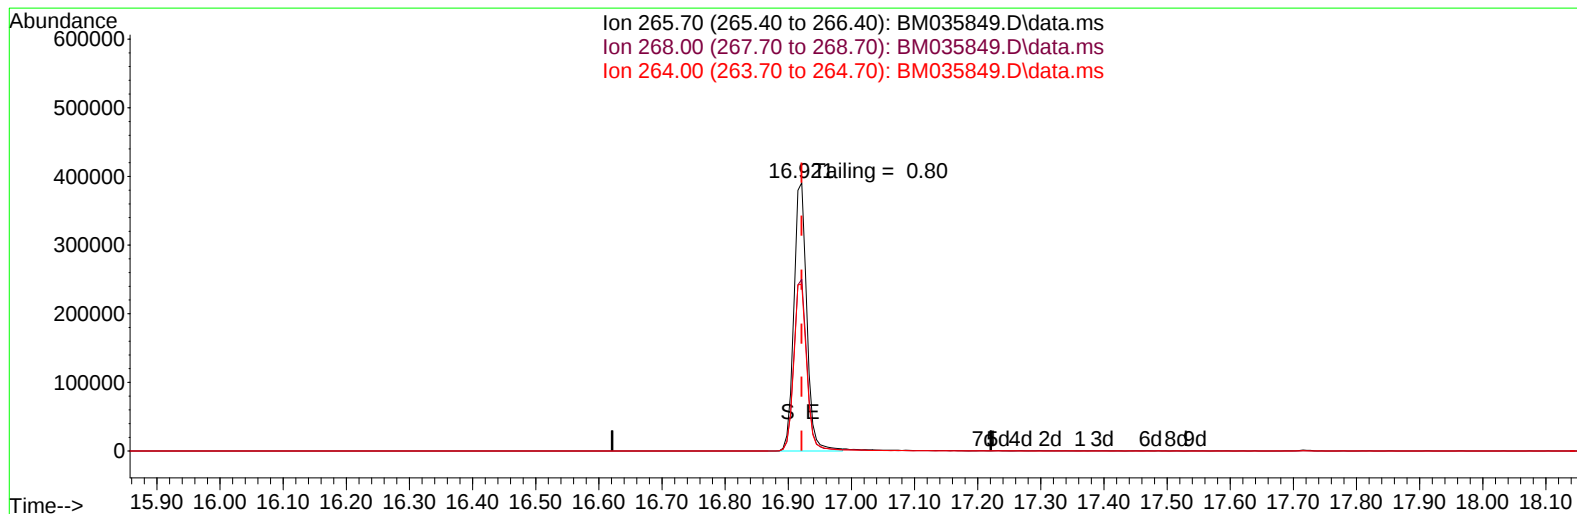

TIC: BM035849.D\data.ms

(70) Pentachlorophenol (C)

16.921min (+ 0.000) 30659.49 ng m




response 567108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.95
264.00	63.30	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071822\
Data File : BM035849.D
Acq On : 18 Jul 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 18 15:03:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 18 14:58:17 2022
Response via : Initial Calibration

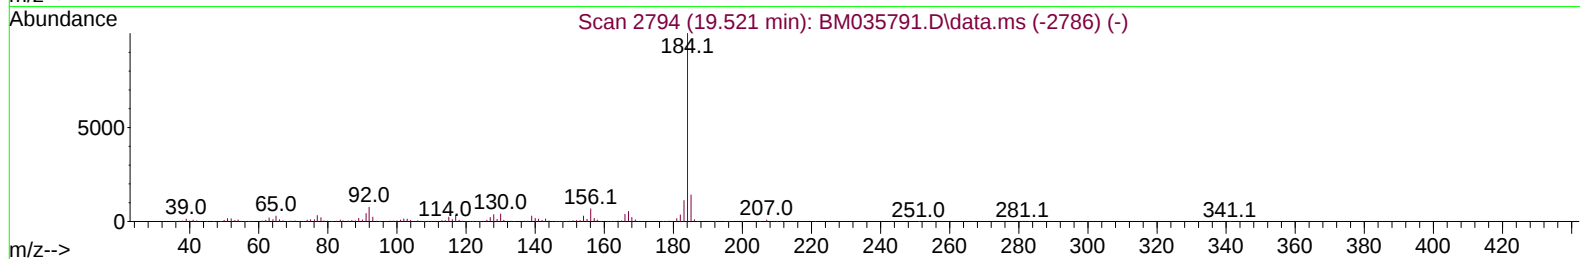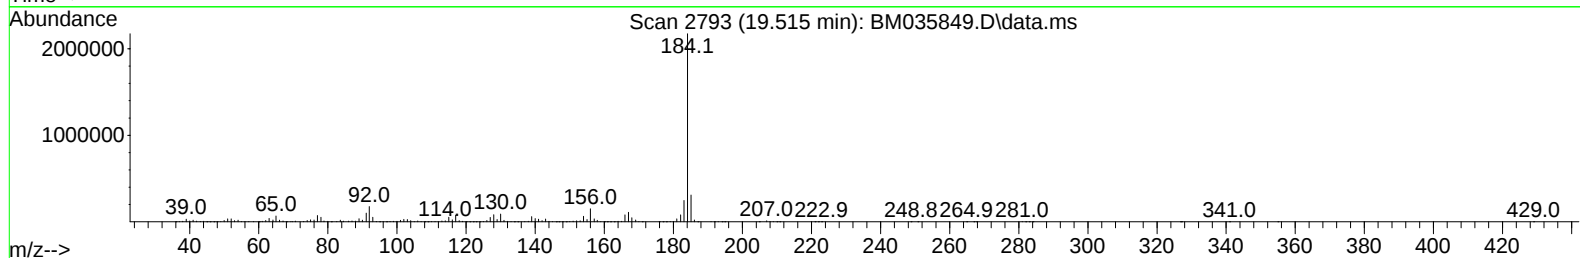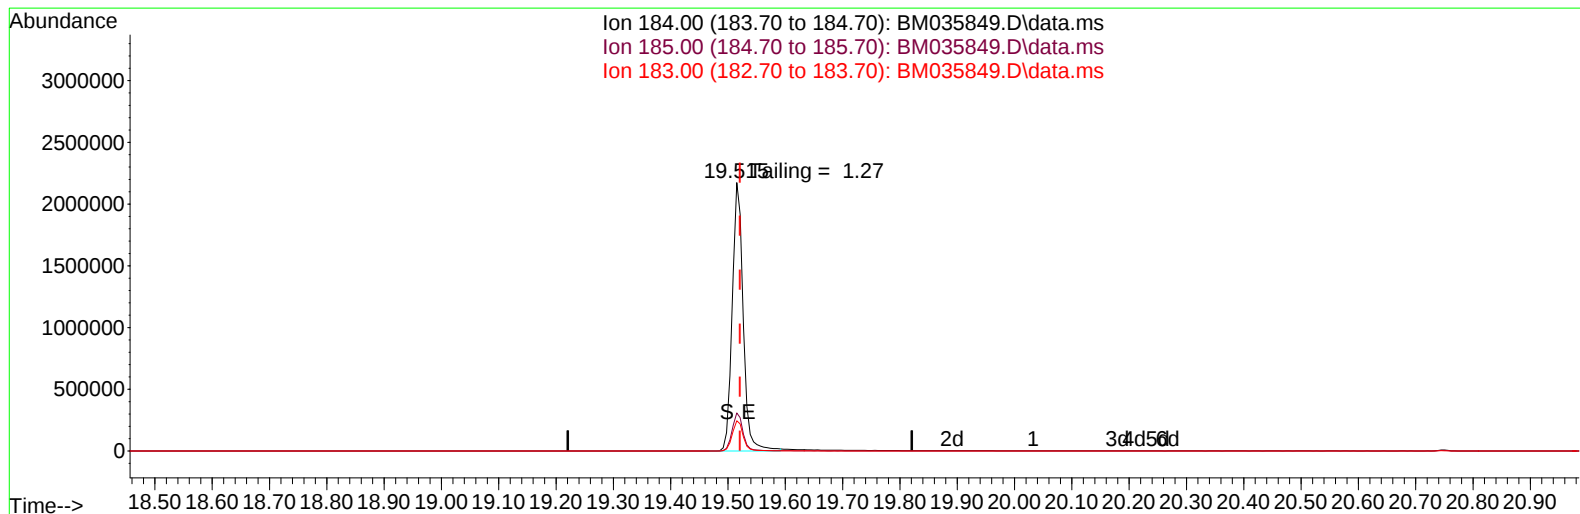

TIC: BM035849.D\data.ms

(77) Benzidine

19.515min (-0.006) 4032843.89 ng m

response 2992345

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.23
183.00	11.90	11.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/18/2022	BNA_M	<u>BM035849.D</u>
Compound Name	Response	Retention Time
DDT	1708277	20.75
DDD	19029	20.3
DDE	2509	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21538	1729815	1.25

Instrument :
BNA_M
ClientSampleId :
DFTPP