
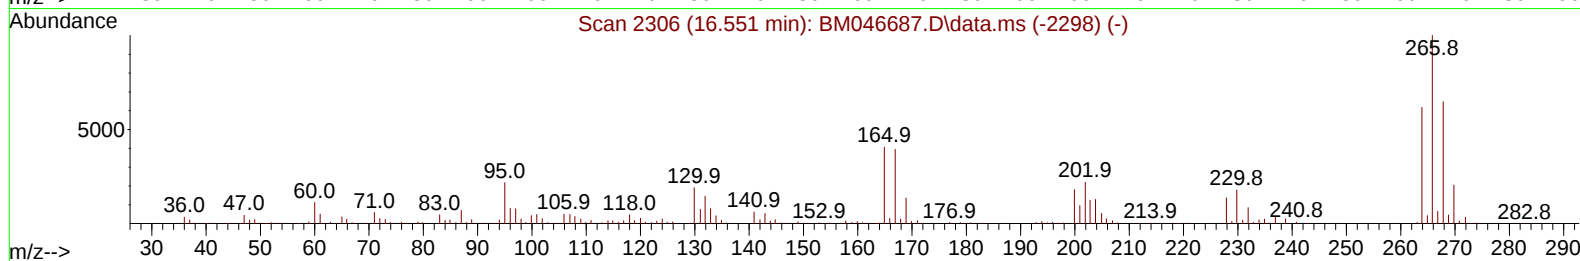
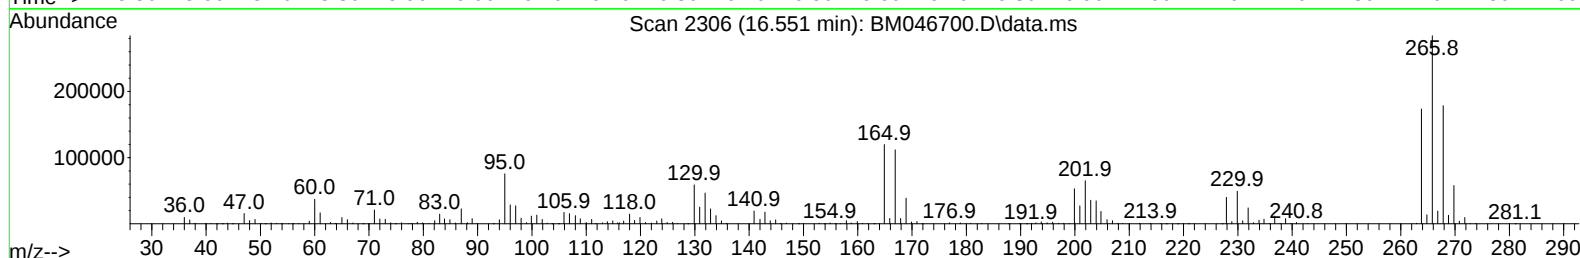


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071824\
Data File : BM046700.D
Acq On : 18 Jul 2024 13:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 14:38:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 18 06:01:46 2024
Response via : Initial Calibration

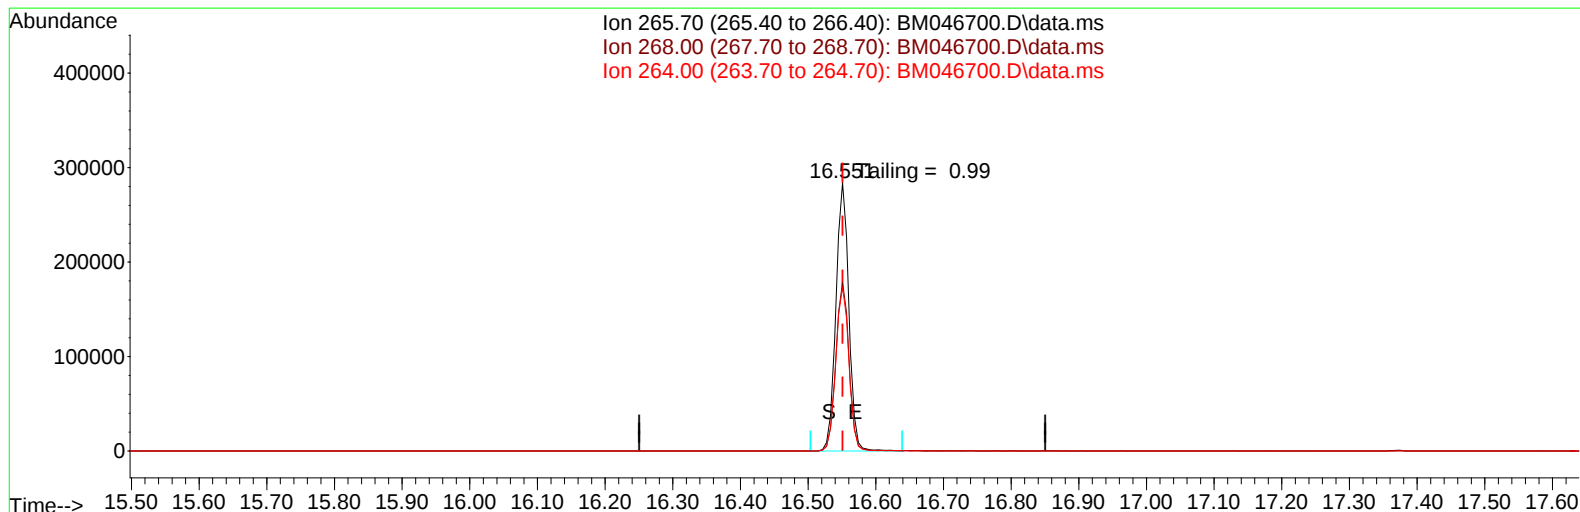

TIC: BM046700.D\data.ms

(70) Pentachlorophenol (C)




16.551min (+ 0.000) 160149.66 ng

response 376600

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	62.87
264.00	61.80	61.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071824\
Data File : BM046700.D
Acq On : 18 Jul 2024 13:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 14:38:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 18 06:01:46 2024
Response via : Initial Calibration

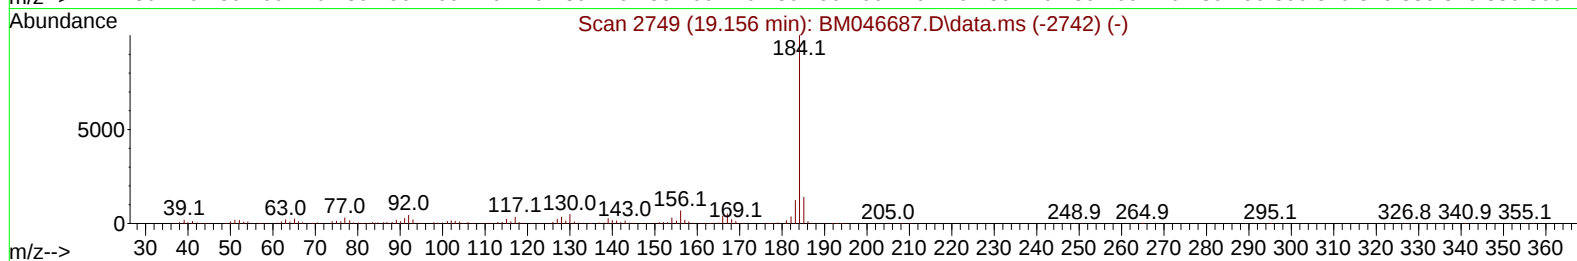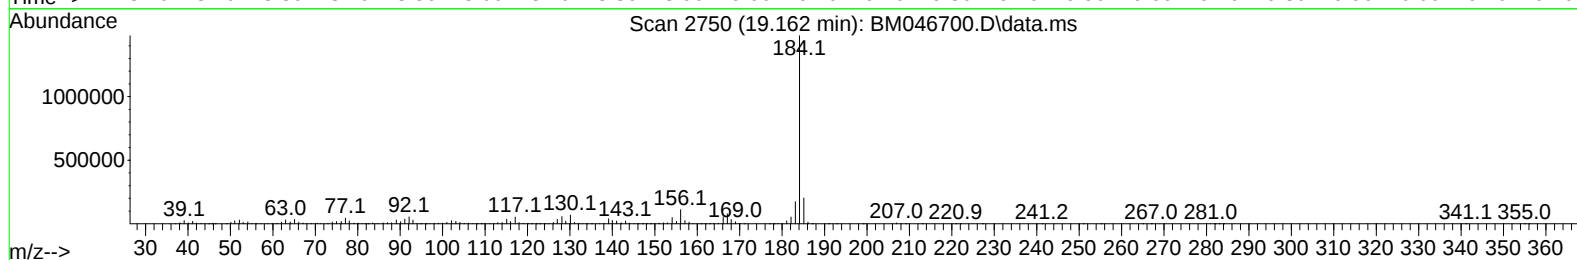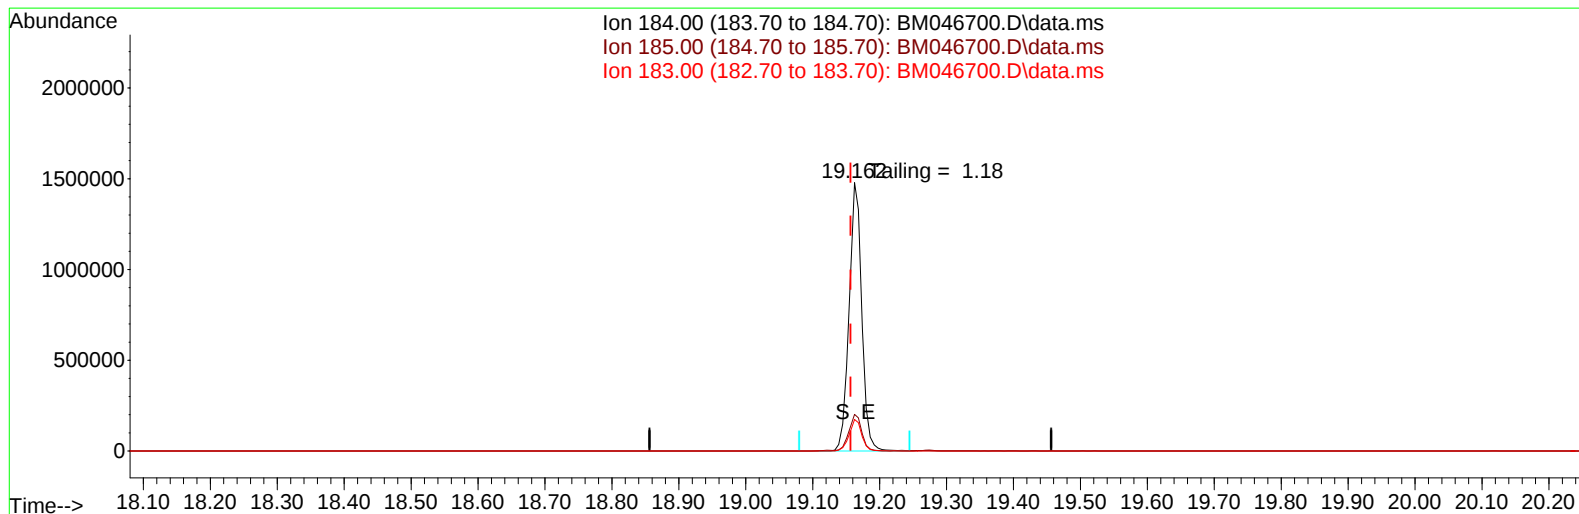

TIC: BM046700.D\data.ms

(77) Benzidine**19.162min (+ 0.006) 48876.34 ng****response 1942348**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.69
183.00	12.30	11.78
0.00	0.00	0.00