


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071824\  
Data File : BM046700.D  
Acq On : 18 Jul 2024 13:09  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071724.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jul 18 06:01:46 2024

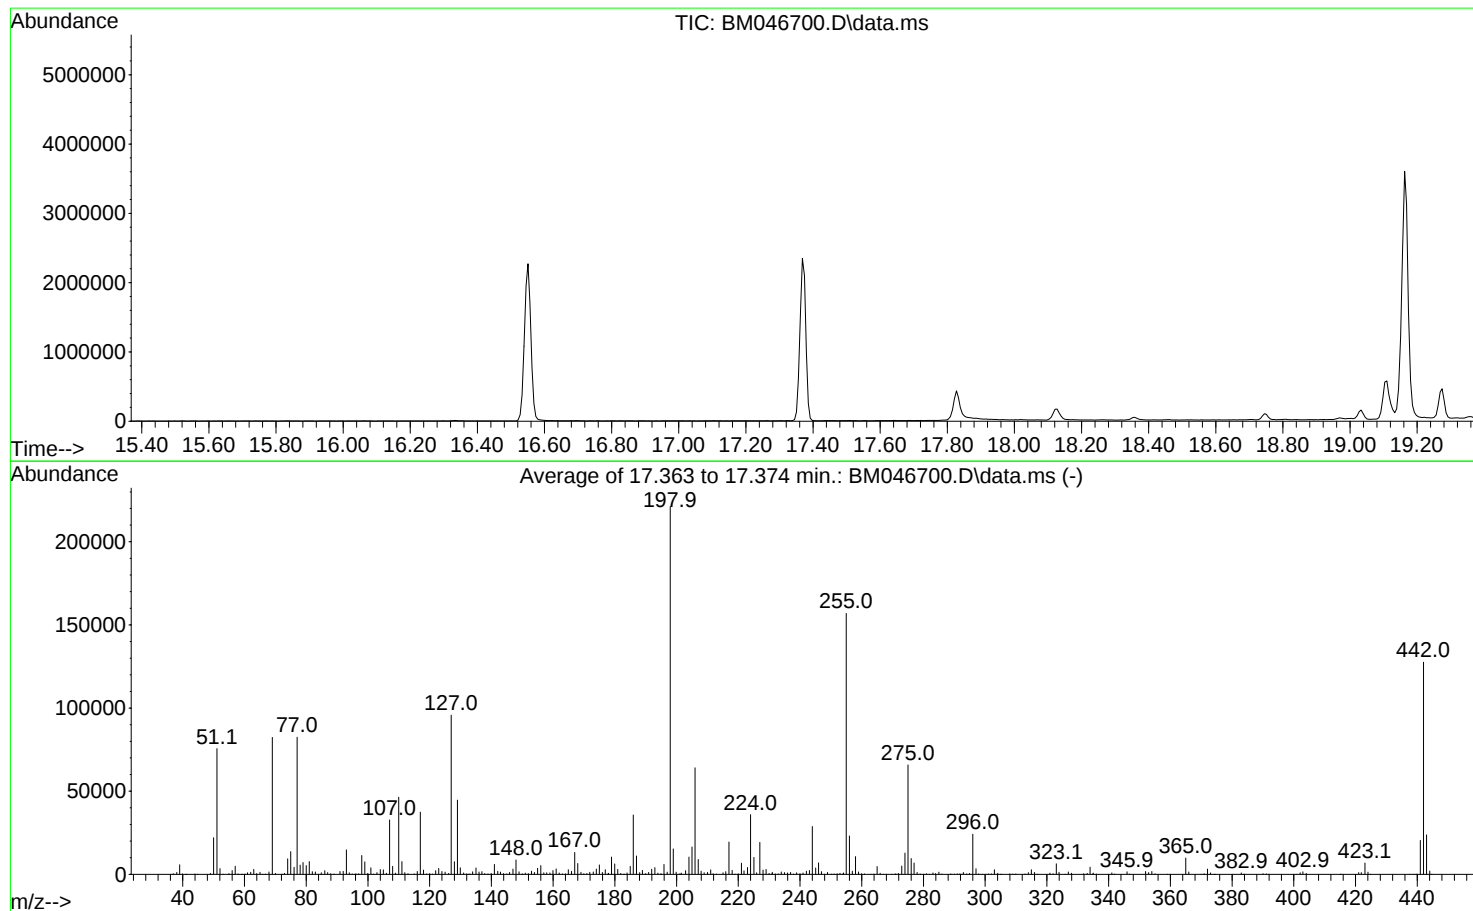




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.2         | 75637      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1463       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.3         | 82401      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 548        | PASS                |
| 127            | 198             | 10              | 80              | 43.3         | 95773      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1383       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 221205     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 15280      | PASS                |
| 275            | 198             | 10              | 60              | 29.8         | 65853      | PASS                |
| 365            | 198             | 1               | 100             | 4.4          | 9812       | PASS                |
| 441            | 198             | 0.01            | 100             | 9.2          | 20436      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 127568     | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 23800      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071824\  
Data File : BM046700.D  
Acq On : 18 Jul 2024 13:09  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jul 18 14:38:32 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 18 06:01:46 2024  
Response via : Initial Calibration

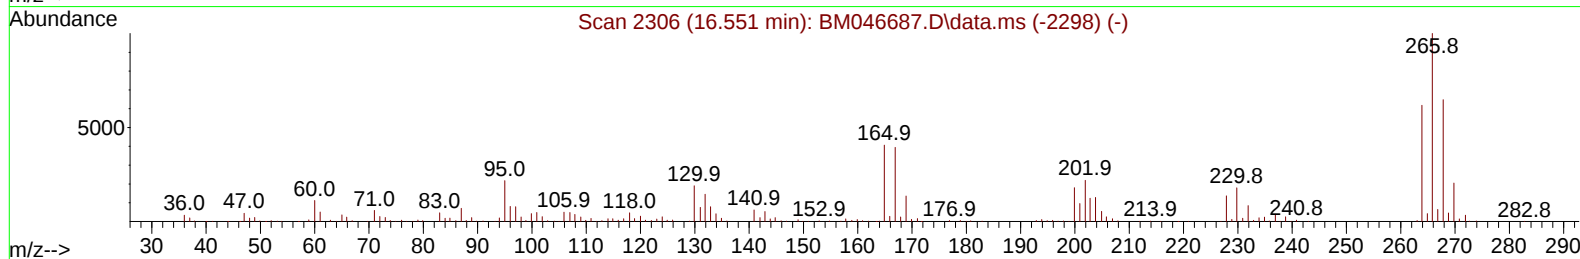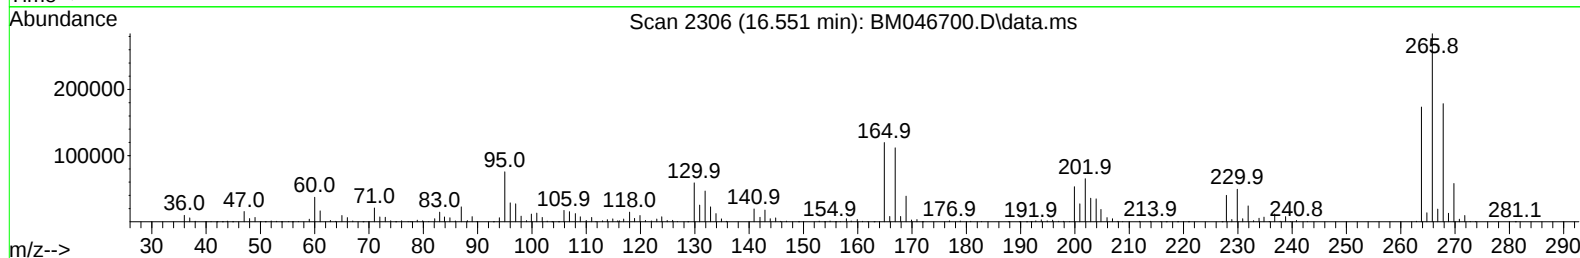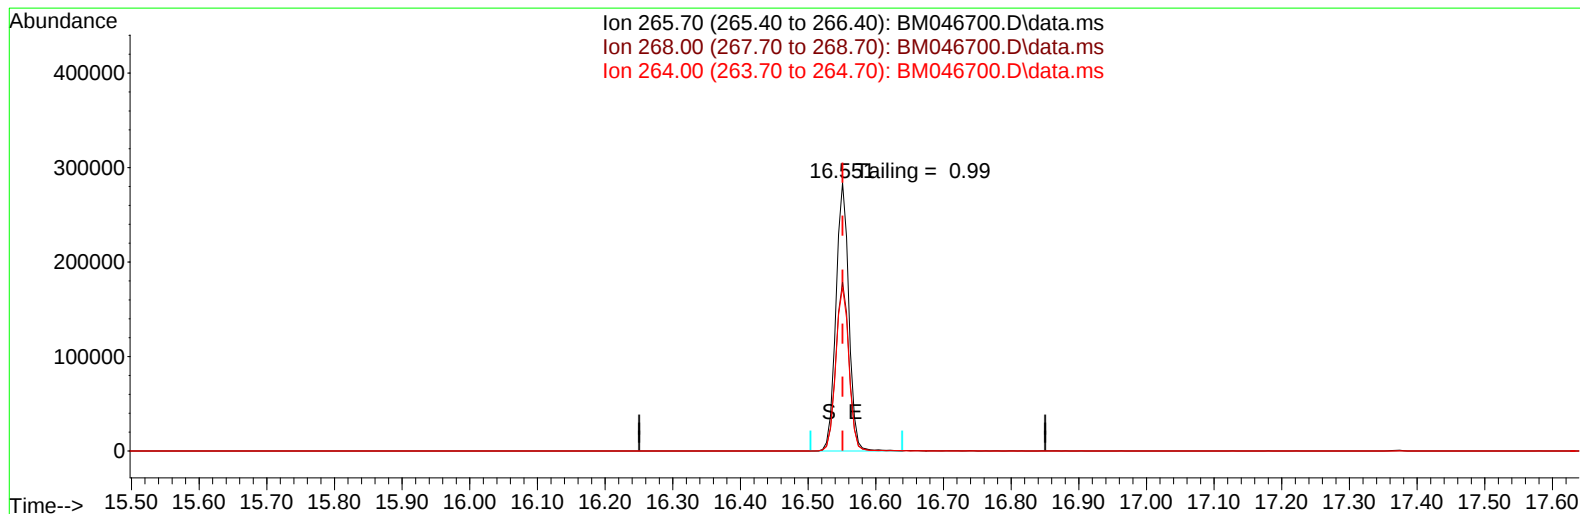

TIC: BM046700.D\data.ms

**(70) Pentachlorophenol (C)**

16.551min (+ 0.000) 160149.66 ng




response 376600

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.80  | 62.87  |
| 264.00 | 61.80  | 61.07  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071824\  
Data File : BM046700.D  
Acq On : 18 Jul 2024 13:09  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jul 18 14:38:32 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 18 06:01:46 2024  
Response via : Initial Calibration

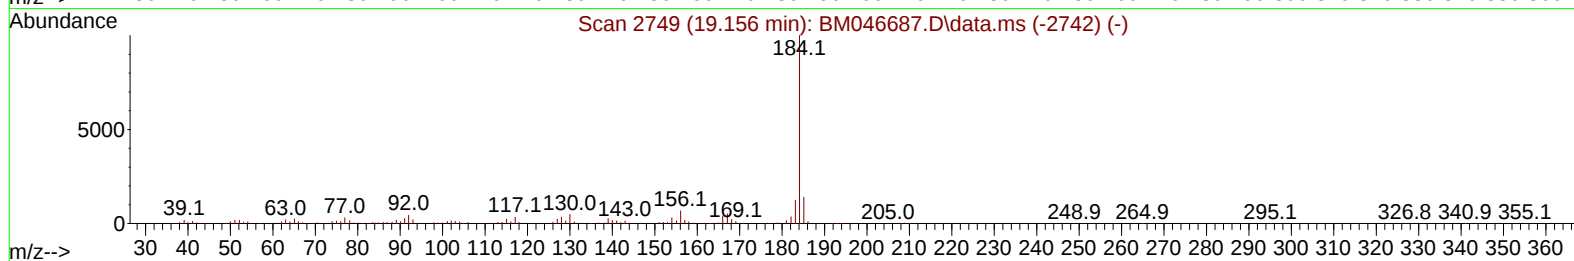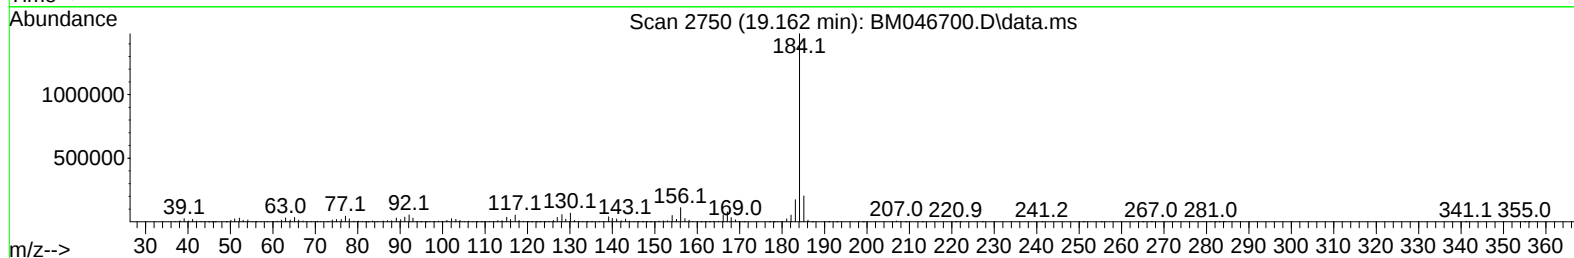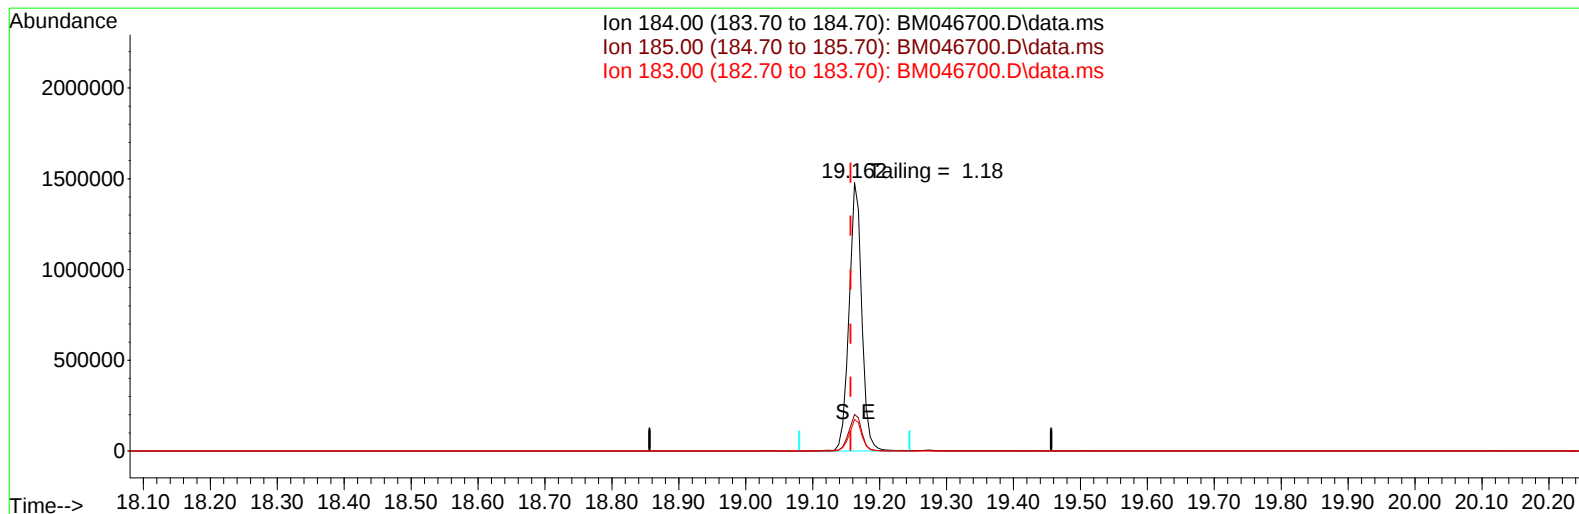

TIC: BM046700.D\data.ms

(77) Benzidine

19.162min (+ 0.006) 48876.34 ng

response 1942348

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.69  |
| 183.00 | 12.30  | 11.78  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/18/2024     | BNA_M            | <u>BM046700.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1186741          | 20.409             |
| DDD           | 17523            | 20.015             |
| DDE           | 1456             | 19.104             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 18979         | 1205720          | 1.57               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP