

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
 Data File : BM006545.D
 Acq On : 20 Jul 2016 05:27
 Operator : UM/SJ
 Sample : H4029-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJB8

Quant Time: Jul 20 05:59:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 20 04:22:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	201619	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	839593	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	464543	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1047185	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1257517	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1329360	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	8545	1.78	ng/uL	0.00
5) Phenol-d5	6.79	99	323692	19.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	205550	20.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	256024	19.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	249890	19.03	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	120832	18.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	130274	18.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	232114	17.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	338389	23.85	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	739696	19.46	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	915466	19.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	117904	17.85	ng/ul	0.00
57) Fluorene-d10	15.26	176	649643	19.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	90596	14.96	ng/ul	0.00
70) Anthracene-d10	17.11	188	1021963	20.65	ng/ul	0.00
76) Pyrene-d10	19.42	212	1184242	20.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1292978	21.27	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	497730	12.90	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006545.D
Acq On : 20 Jul 2016 05:27
Operator : UM/SJ
Sample : H4029-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB8

Quant Time: Jul 20 05:59:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 20 04:22:37 2016
Response via : Initial Calibration

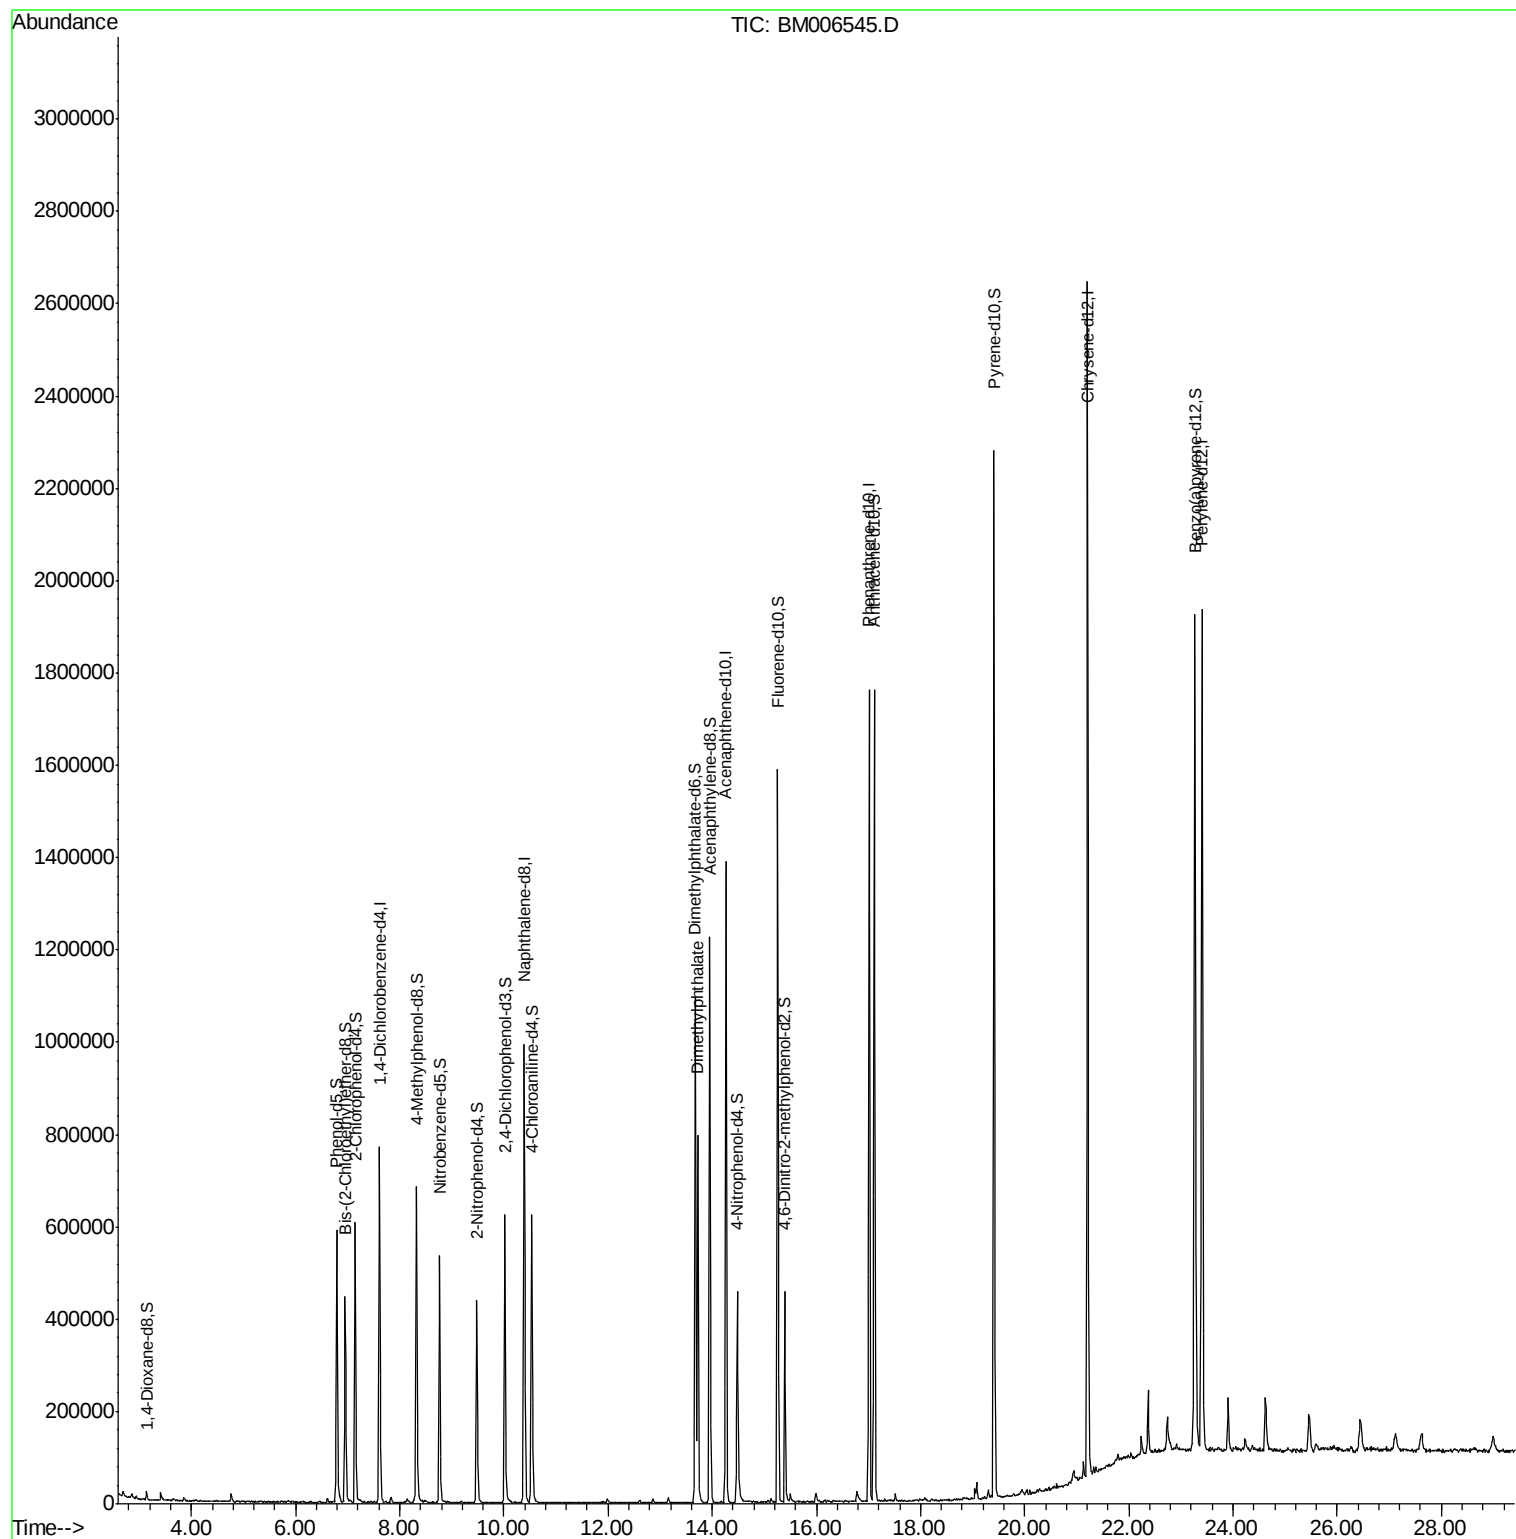

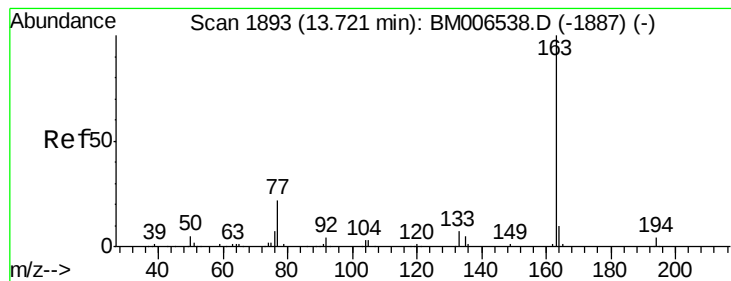

#44

Dimethylphthalate

Concen: 12.90 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006545.D


Acq: 20 Jul 2016 05:27

Instrument :

BNA_M

ClientSampleId :

BDJB8

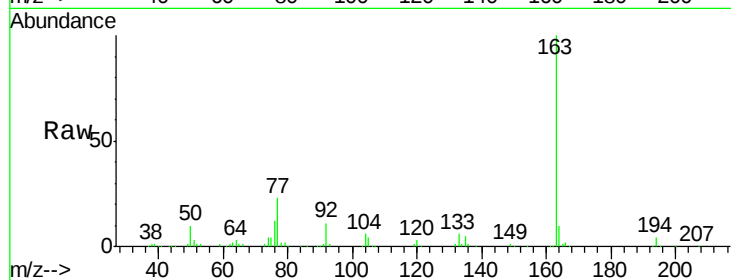

Tgt Ion:163 Resp: 497730

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.2 7.8 11.8

