

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
 Data File : BM006548.D
 Acq On : 20 Jul 2016 09:30
 Operator : UM/SJ
 Sample : H3959-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ22

Manual Integrations

sohil
 7/20/2016 7:48:09 PM

Quant Time: Jul 20 13:57:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 20 04:22:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	190962	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	793804	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	433393	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	962699	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1033034	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1190290	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	6509	1.44	ng/uL	0.00
5) Phenol-d5	6.79	99	254118	16.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	170031	17.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	203427	16.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	203087	16.33	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	96587	16.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	104166	15.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	188105	14.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	265090	19.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	572960	16.15	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	728899	16.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	61201	9.93	ng/ul	0.00
57) Fluorene-d10	15.26	176	519834	16.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	41197	7.40	ng/ul	0.00
70) Anthracene-d10	17.12	188	767875	16.87	ng/ul	0.00
76) Pyrene-d10	19.42	212	829654	17.71	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	924266	16.98	ng/ul	0.00

Target Compounds

					Qvalue
28) Naphthalene	10.46	128	10204413	253.27 ng/ul	99
34) 2-Methylnaphthalene	12.06	142	1114462	36.71 ng/ul	98
40) 1,1'-Biphenyl	13.09	154	323395	9.05 ng/ul	100
44) Dimethylphthalate	13.72	163	113447	3.15 ng/ul	99
47) Acenaphthylene	13.98	152	158471	3.47 ng/ul#	96
49) Acenaphthene	14.33	153	1870371	63.65 ng/ul	98
53) Dibenzofuran	14.67	168	1432418	33.48 ng/ul	100
58) Fluorene	15.32	166	1428134	41.74 ng/ul	100
69) Phenanthrene	17.06	178	5500055	103.90 ng/ul	98
71) Anthracene	17.15	178	2114792	38.84 ng/ul	99
72) Carbazole	17.42	167	367102	7.97 ng/ul	98
74) Fluoranthene	19.09	202	5030406	81.77 ng/ul	96
77) Pyrene	19.45	202	4140348	67.13 ng/ul	96
80) Benzo(a)anthracene	21.20	228	2059388	32.66 ng/ul	97
82) Chrysene	21.25	228	1781389	30.01 ng/ul	98
85) Benzo(b)fluoranthene	22.76	252	2392820	33.64 ng/ul	98
86) Benzo(k)fluoranthene	22.79	252	689623m	10.31 ng/ul	
88) Benzo(a)pyrene	23.31	252	1700471	24.96 ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.60	276	1062090	13.40 ng/ul	96
90) Dibenzo(a,h)anthracene	25.60	278	282769	4.29 ng/ul#	83
91) Benzo(g,h,i)perylene	26.27	276	861455	12.29 ng/ul	99

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006548.D
Acq On : 20 Jul 2016 09:30
Operator : UM/SJ
Sample : H3959-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ22

Manual Integrations

sohil
7/20/2016 7:48:09 PM

Quant Time: Jul 20 13:57:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 20 04:22:37 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006548.D
Acq On : 20 Jul 2016 09:30
Operator : UM/SJ
Sample : H3959-03
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJ22

Manual Integrations

sohil
7/20/2016 7:48:09 PM

Quant Time: Jul 20 13:57:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 20 04:22:37 2016
Response via : Initial Calibration

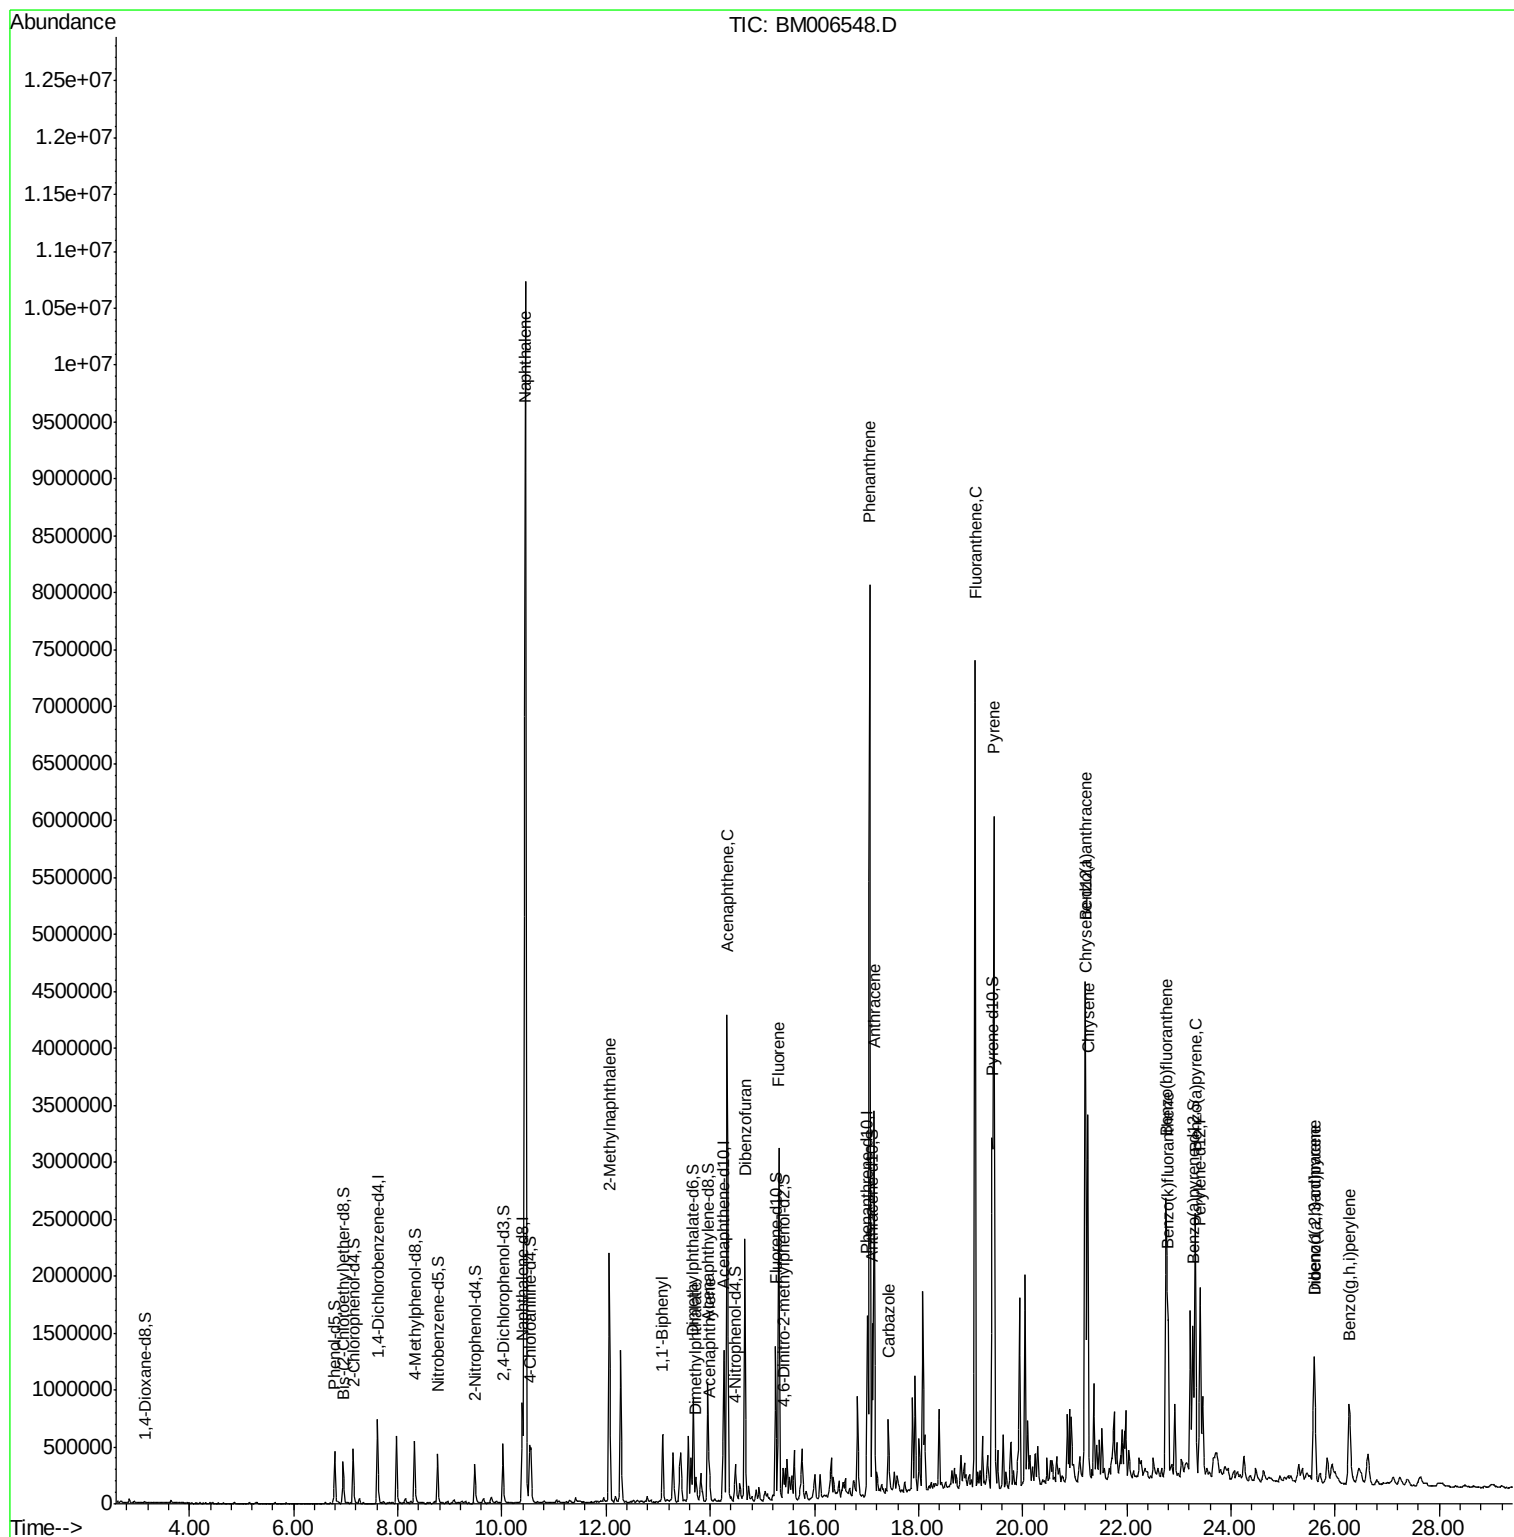

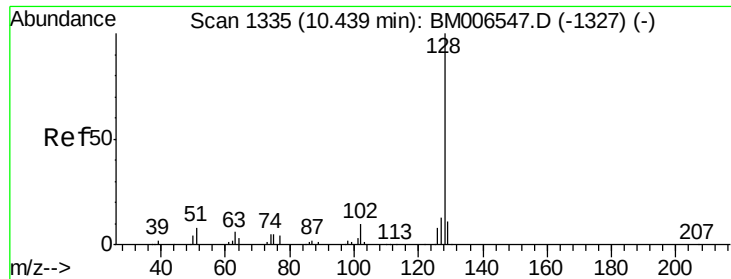





#28
Naphthalene
Concen: 253.27 ng/ul
RT: 10.46 min Scan# 1338
Delta R.T. 0.02 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Instrument :
BNA_M
ClientSampleId :
BDJ22

Tgt Ion:128 Resp:10204413
Ion Ratio Lower Upper
128 100
129 11.1 8.6 13.0
127 13.9 10.9 16.3




Manual Integrations


sohil
7/20/2016 7:48:09 PM

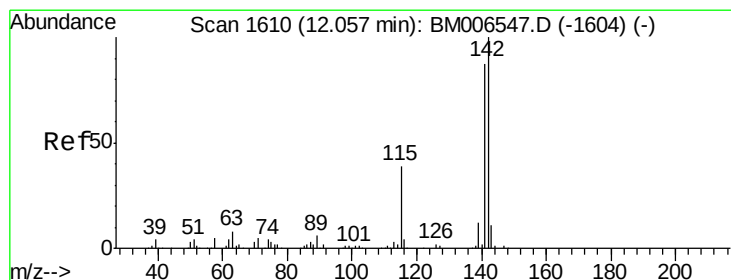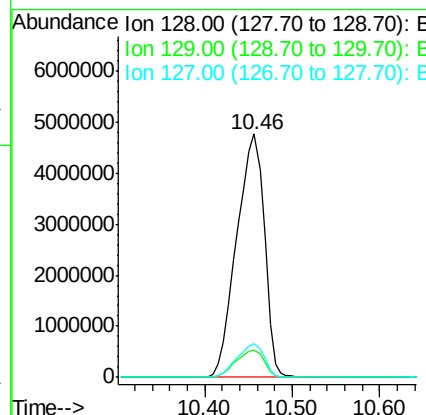

#34
2-Methylnaphthalene
Concen: 36.71 ng/ul
RT: 12.06 min Scan# 1611
Delta R.T. 0.00 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Tgt Ion:142 Resp: 1114462
Ion Ratio Lower Upper
142 100
141 87.9 69.0 103.4

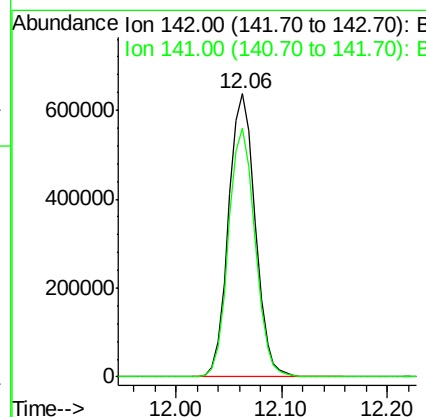

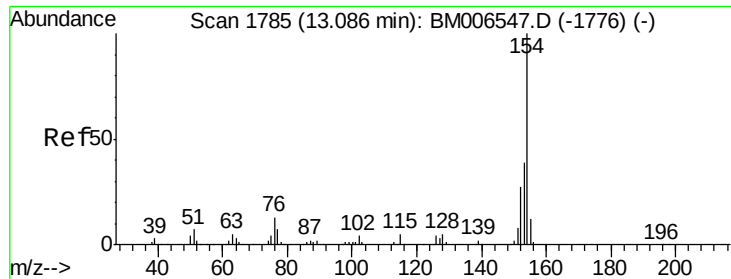

#40

1,1'-Biphenyl

Concen: 9.05 ng/ul

RT: 13.09 min Scan# 1785

Delta R.T. -0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30

Instrument :

BNA_M

ClientSampled :


BDJ22

Tgt Ion:	154	Resp:	323395
Ion Ratio	Lower	Upper	
154	100		
153	39.2	31.4	47.2
76	13.4	10.4	15.6

Manual Integrations

sohil




7/20/2016 7:48:09 PM



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

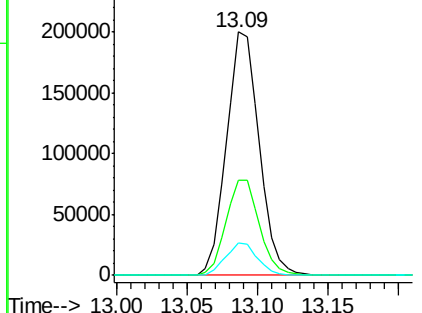

#44

Dimethylphthalate

Concen: 3.15 ng/ul


RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30



Tgt Ion:	163	Resp:	113447
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.4	5.0
164	10.3	7.8	11.8




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

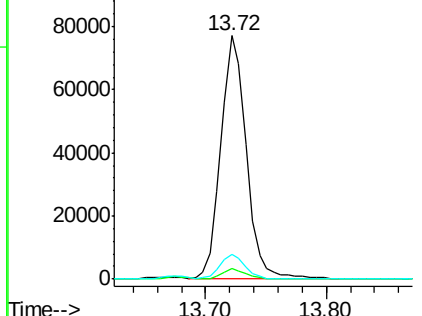

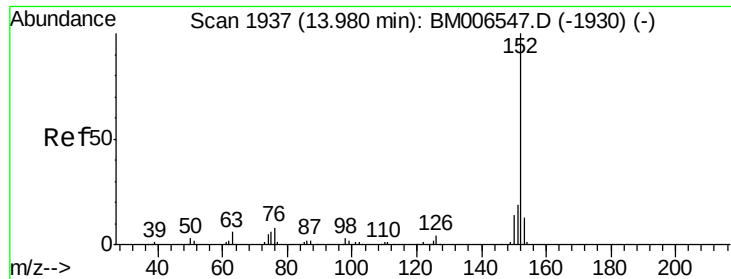





#47
Acenaphthylene
Concen: 3.47 ng/ul
RT: 13.98 min Scan# 1937
Delta R.T. -0.01 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Instrument :
BNA_M
ClientSampled :
BDJ22

Tgt Ion	Ratio	Lower	Upper
152	100		
151	18.8	15.6	23.4
153	15.9	10.3	15.5#




Manual Integrations


sohil
7/20/2016 7:48:09 PM

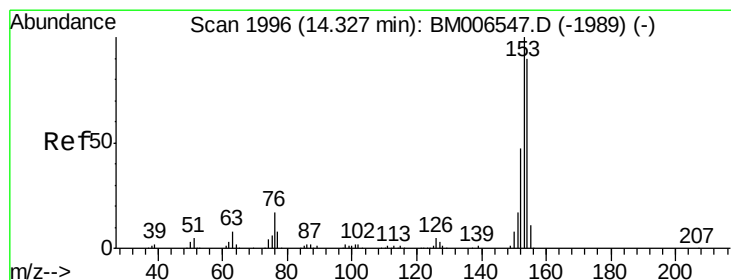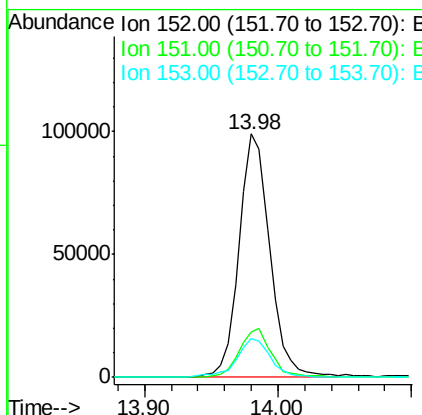

#49
Acenaphthene
Concen: 63.65 ng/ul
RT: 14.33 min Scan# 1996
Delta R.T. -0.00 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Tgt Ion	Ratio	Lower	Upper
153	100		
152	48.1	37.7	56.5
154	90.1	70.0	105.0

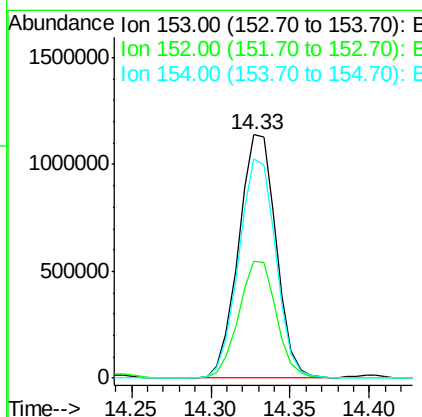

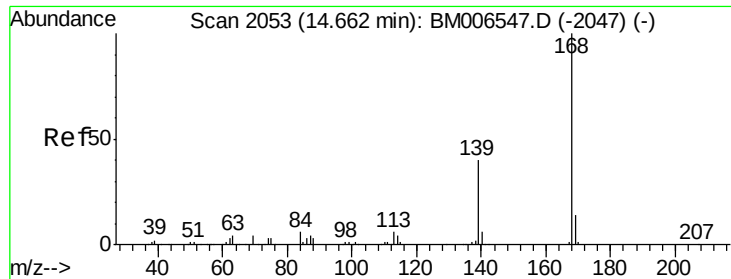

#53

Dibenzenofuran

Concen: 33.48 ng/ul

RT: 14.67 min Scan# 2054

Delta R.T. 0.00 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30

Instrument :

BNA_M

ClientSampled :

BDJ22

Tgt Ion:168 Resp: 1432418

Ion Ratio Lower Upper





168 100

139 38.5 30.6 46.0

Manual Integrations

sohil

7/20/2016 7:48:09 PM

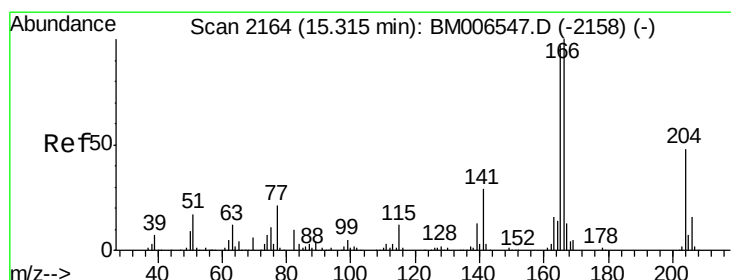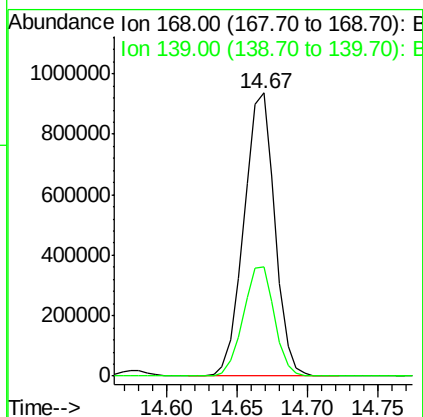

#58

Fluorene

Concen: 41.74 ng/ul

RT: 15.32 min Scan# 2164

Delta R.T. -0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30




Tgt Ion:166 Resp: 1428134


Ion Ratio Lower Upper

166 100

165 97.1 77.5 116.3

167 13.7 10.8 16.2

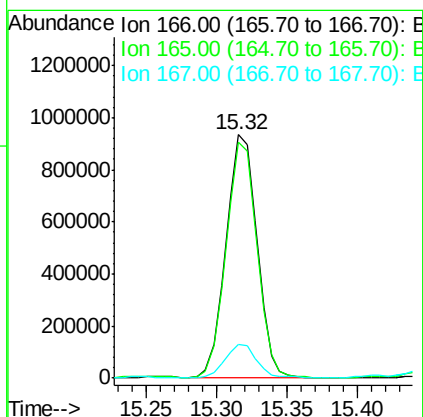



#69

Phenanthrene

Concen: 103.90 ng/ul

RT: 17.06 min Scan# 2461

Delta R.T. 0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30

Instrument :

BNA_M

ClientSampleId :

BDJ22

Tgt Ion:178 Resp: 5500055

Ion Ratio Lower Upper

178 100


179 15.7 11.9 17.9

176 20.0 15.2 22.8

Manual Integrations

sohil




7/20/2016 7:48:09 PM

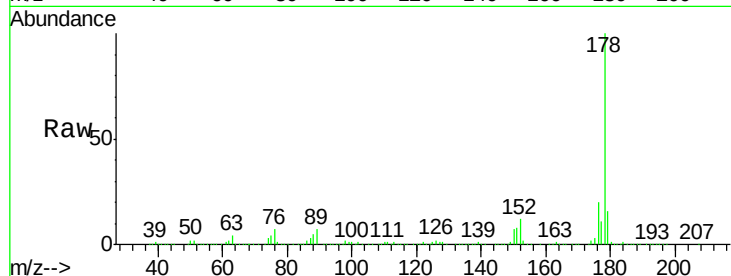

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

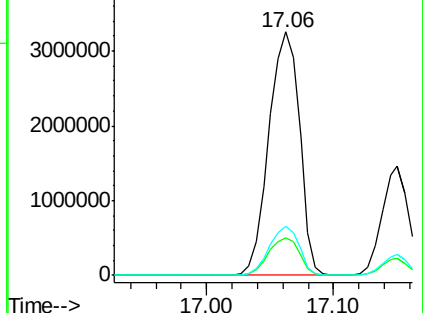

#71

Anthracene

Concen: 38.84 ng/ul

RT: 17.15 min Scan# 2476

Delta R.T. 0.00 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30


Tgt Ion:178 Resp: 2114792

Ion Ratio Lower Upper

178 100

179 15.5 12.0 18.0



176 18.8 15.0 22.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

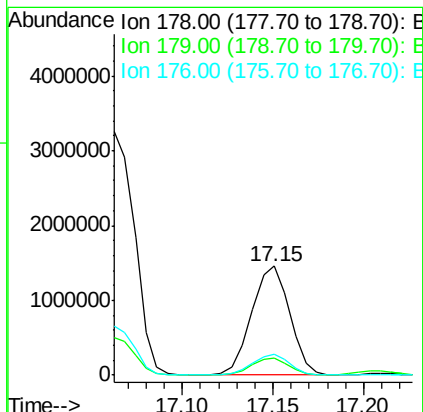

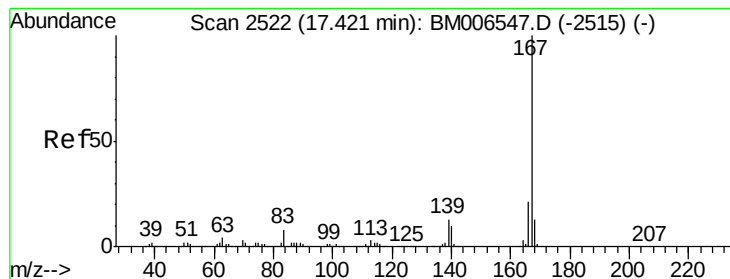

#72

Carbazole

Concen: 7.97 ng/ul

RT: 17.42 min Scan# 2522

Delta R.T. -0.00 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30

Instrument :

BNA_M

ClientSampleId :


BDJ22

Tgt Ion:	167	Resp:	367102
Ion Ratio	Lower	Upper	
167	100		
166	22.1	17.0	25.6
139	13.7	10.2	15.4

Manual Integrations

sohil




7/20/2016 7:48:09 PM

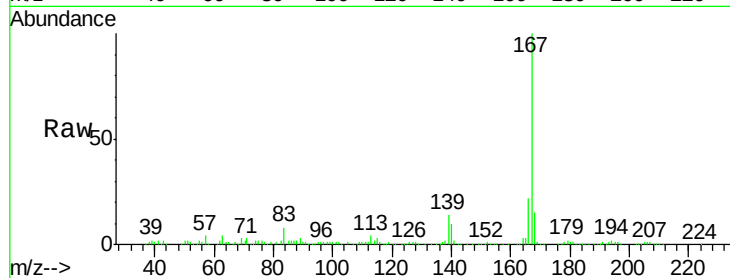

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

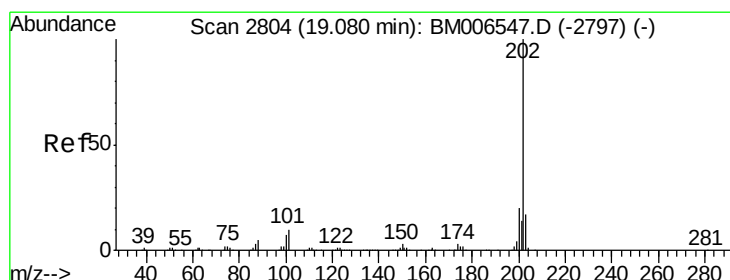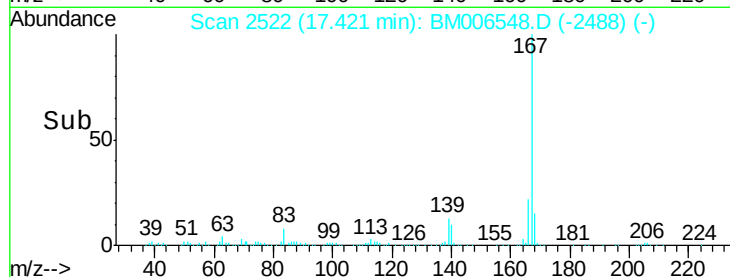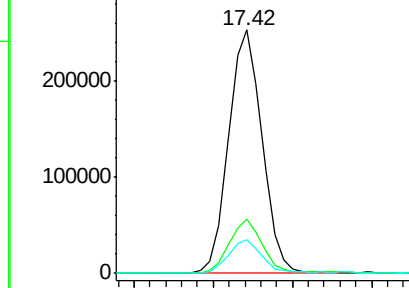

#74

Fluoranthene

Concen: 81.77 ng/ul


RT: 19.09 min Scan# 2805

Delta R.T. 0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30



Tgt Ion:	202	Resp:	5030406
Ion Ratio	Lower	Upper	
202	100		
101	9.0	8.6	12.8
100	6.5	6.4	9.6

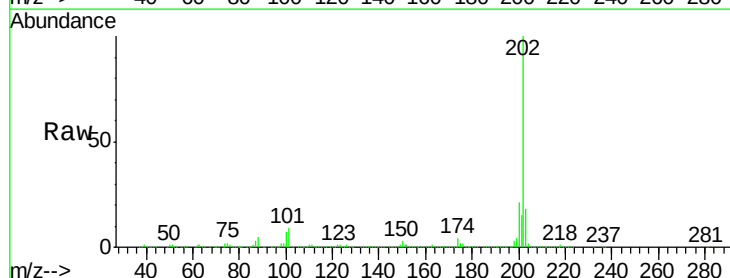


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

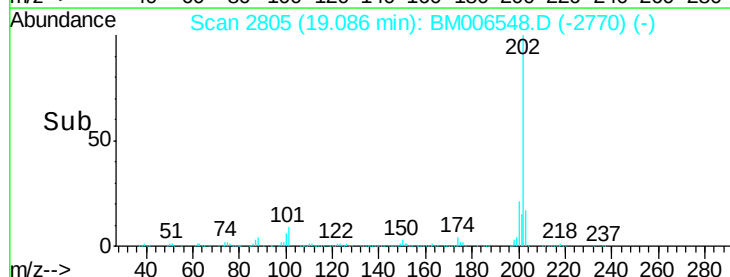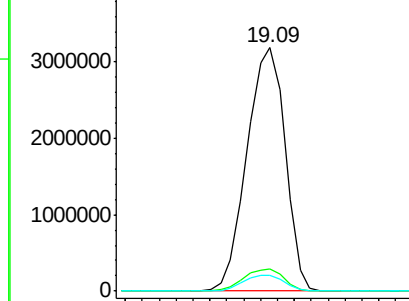

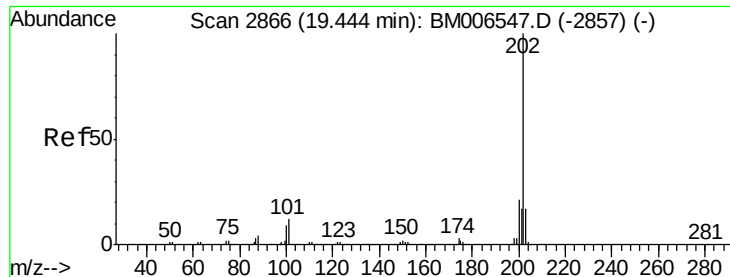

#77

Pyrene

Concen: 67.13 ng/ul

RT: 19.45 min Scan# 2867

Delta R.T. 0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30

Instrument :

BNA_M

ClientSampleId :

BDJ22

Tgt Ion:202 Resp: 4140348

Ion Ratio Lower Upper

202 100


101 11.0 10.0 15.0

100 8.6 7.9 11.9

Manual Integrations

sohil




7/20/2016 7:48:09 PM

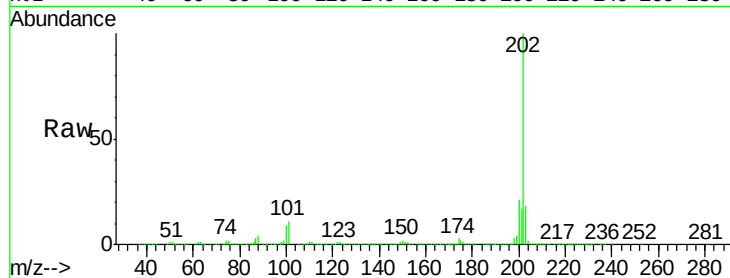

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

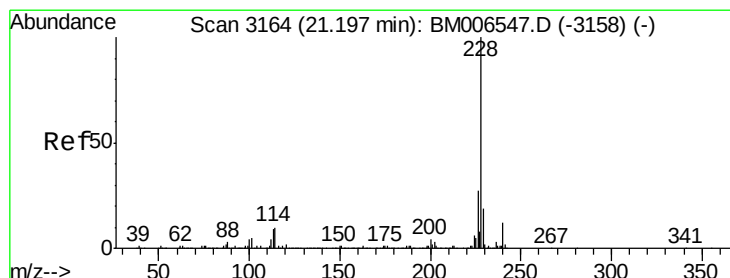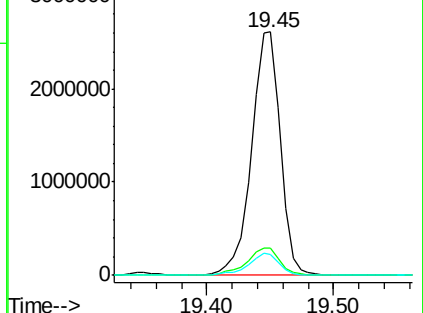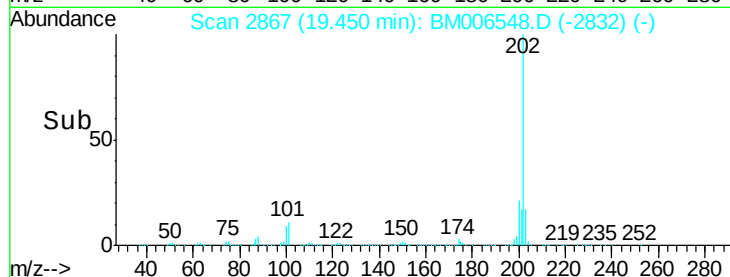

#80

Benzo(a)anthracene

Concen: 32.66 ng/ul

RT: 21.20 min Scan# 3164

Delta R.T. 0.00 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30


Tgt Ion:228 Resp: 2059388

Ion Ratio Lower Upper

228 100

229 20.1 15.6 23.4



226 28.8 21.4 32.2

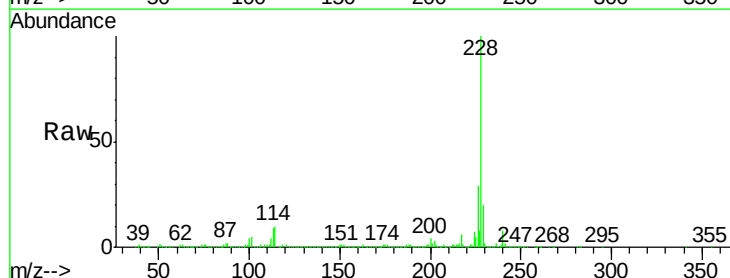


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

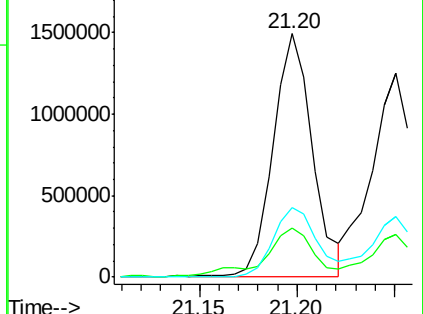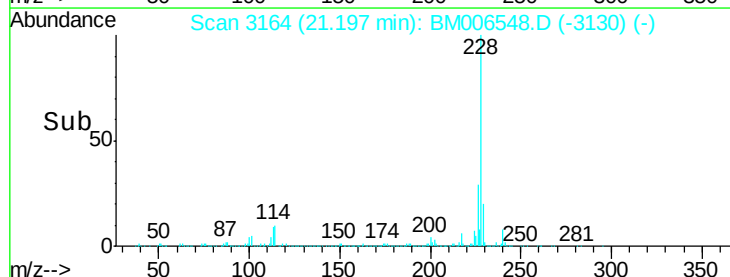

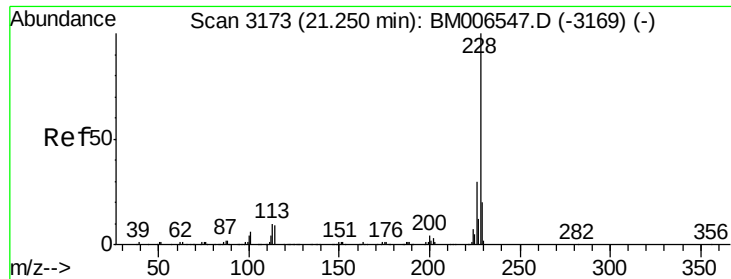


#82
Chrysene
Concen: 30.01 ng/ul
RT: 21.25 min Scan# 3173
Delta R.T. 0.00 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Instrument :
BNA_M
ClientSampleId :
BDJ22




Tgt Ion:228 Resp: 1781389
Ion Ratio Lower Upper
228 100
226 30.0 23.3 34.9
229 20.9 15.8 23.8

Manual Integrations

sohil
7/20/2016 7:48:09 PM




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

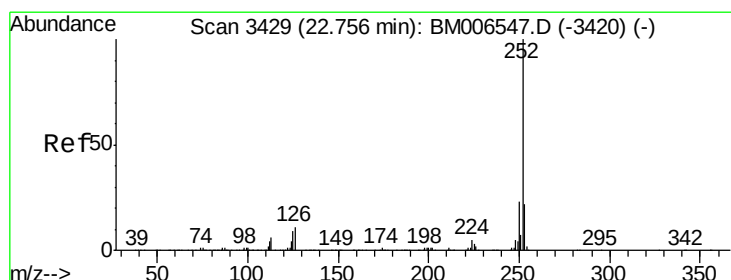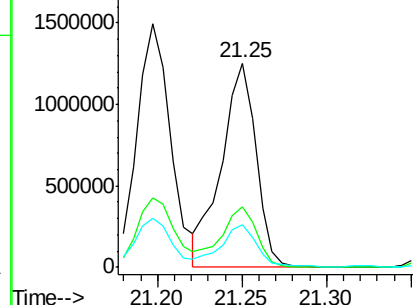




#85
Benzo(b)fluoranthene
Concen: 33.64 ng/ul
RT: 22.76 min Scan# 3429
Delta R.T. 0.00 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Tgt Ion:252 Resp: 2392820
Ion Ratio Lower Upper
252 100
253 22.4 17.4 26.2
125 9.6 6.7 10.1

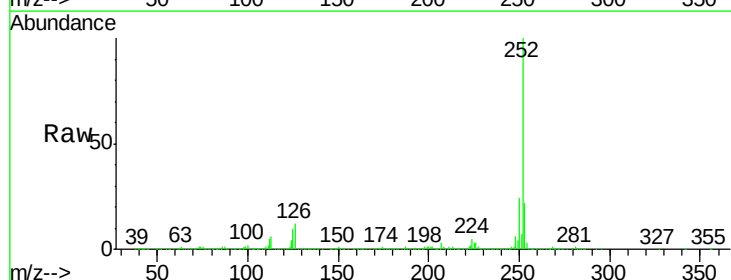

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

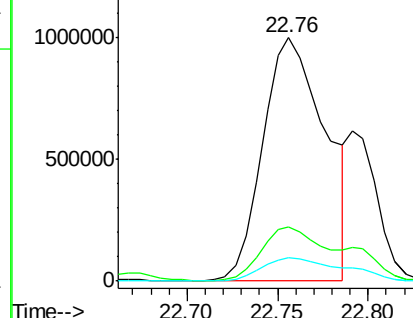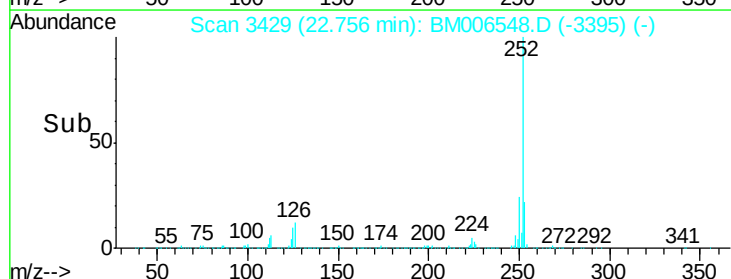

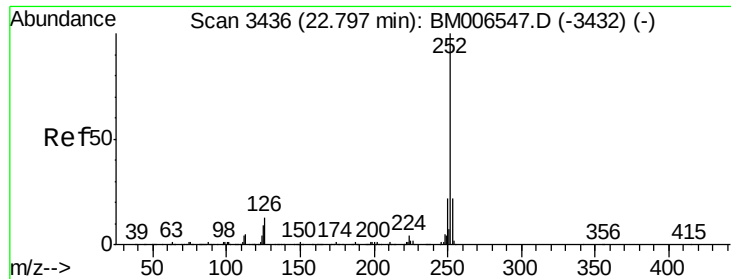





#86
Benzo(k)fluoranthene
Concen: 10.31 ng/ul m
RT: 22.79 min Scan# 3435
Delta R.T. -0.01 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Instrument :
BNA_M
ClientSampleId :
BDJ22

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.3	25.9
125	9.0	7.0	10.4




Manual Integrations


sohil
7/20/2016 7:48:09 PM

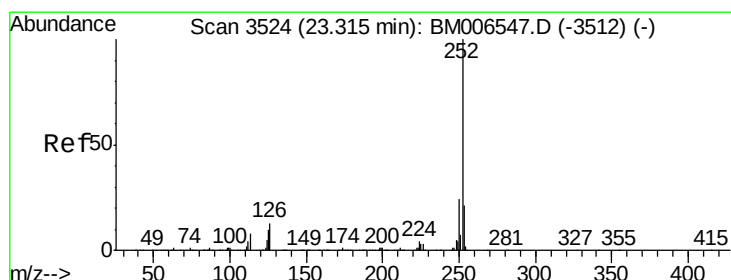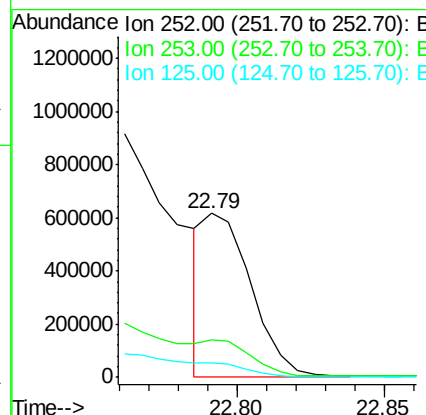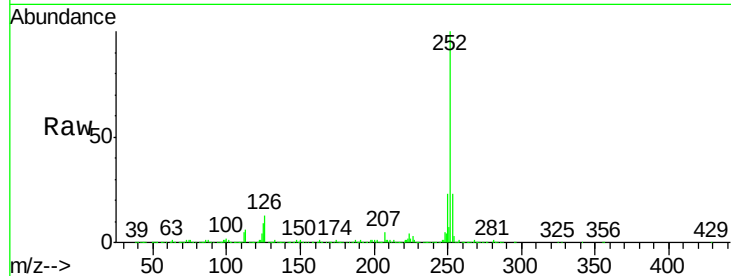

#88
Benzo(a)pyrene
Concen: 24.96 ng/ul
RT: 23.31 min Scan# 3524
Delta R.T. -0.01 min
Lab File: BM006548.D
Acq: 20 Jul 2016 09:30

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.0	17.4	26.2
125	9.9	7.6	11.4

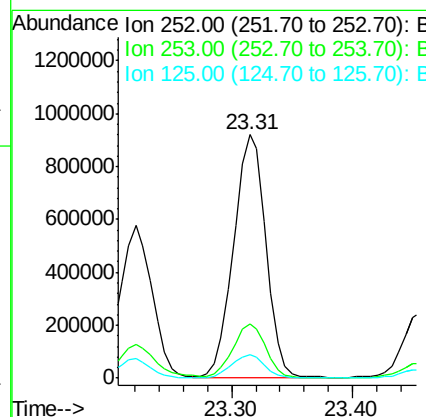

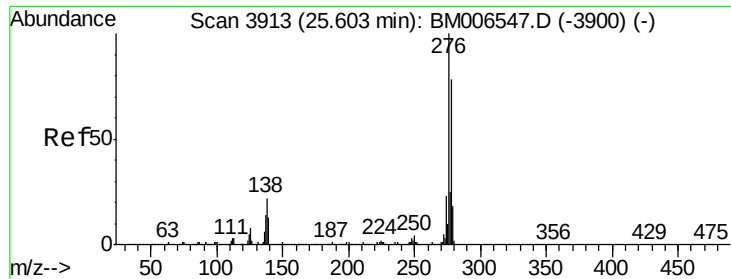





#89
 Indeno(1,2,3-cd)pyrene
 Concen: 13.40 ng/ul
 RT: 25.60 min Scan# 3913
 Delta R.T. -0.01 min
 Lab File: BM006548.D
 Acq: 20 Jul 2016 09:30

Instrument :
 BNA_M
 ClientSampleId :
 BDJ22

Tgt Ion: 276 Resp: 1062090
 Ion Ratio Lower Upper
 276 100
 138 18.5 17.8 26.6
 277 24.5 20.1 30.1




Manual Integrations




sohil
 7/20/2016 7:48:09 PM

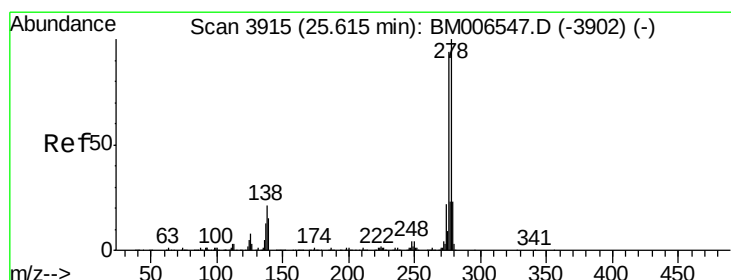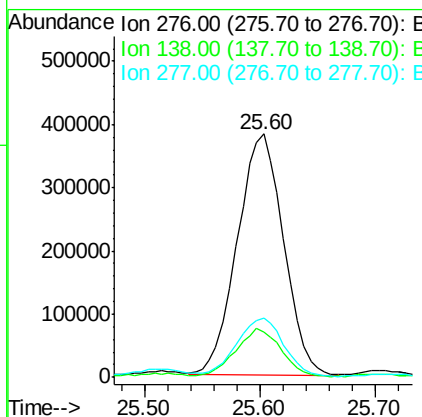

#90
 Dibenzo(a,h)anthracene
 Concen: 4.29 ng/ul
 RT: 25.60 min Scan# 3913
 Delta R.T. -0.02 min
 Lab File: BM006548.D
 Acq: 20 Jul 2016 09:30

Tgt Ion: 278 Resp: 282769
 Ion Ratio Lower Upper
 278 100
 139 0.0 11.7 17.5#
 279 27.2 19.2 28.8

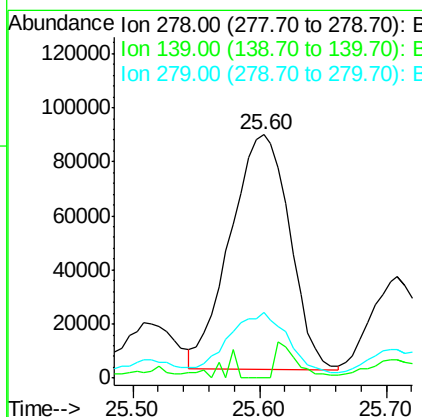

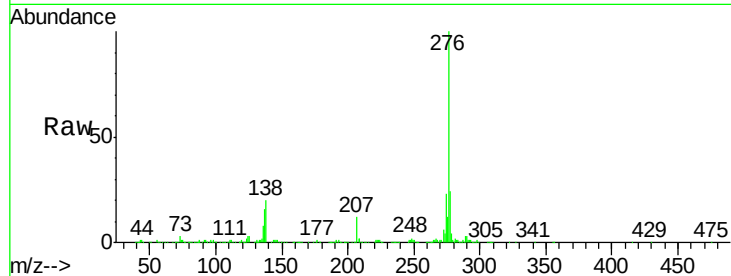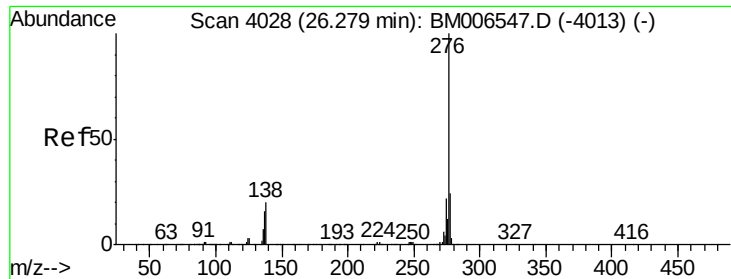

#91

Benzo(g,h,i)perylene

Concen: 12.29 ng/ul

RT: 26.27 min Scan# 4027

Delta R.T. -0.01 min

Lab File: BM006548.D

Acq: 20 Jul 2016 09:30

Instrument :

BNA_M

ClientSampleId :

BDJ22

Tgt Ion: 276 Resp: 861455

Ion Ratio Lower Upper

276 100

138 19.7 15.0 22.4

277 24.1 19.0 28.4

Manual Integrations

sohil

7/20/2016 7:48:09 PM

