

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
 Data File : BM006526.D
 Acq On : 19 Jul 2016 17:21
 Operator : UM/SJ
 Sample : H4029-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	726	rBV	248162	416522	12.56%	1.259%
2	6.958	737	743	755	rBV	193685	319258	9.63%	0.965%
3	7.146	769	775	788	rVB	245452	416979	12.57%	1.261%
4	7.616	848	855	866	rBV	598720	990896	29.88%	2.996%
5	8.322	969	975	990	rBV	274143	472915	14.26%	1.430%
6	8.769	1045	1051	1061	rBV	222034	391107	11.79%	1.183%
7	9.487	1166	1173	1185	rBV	172941	305862	9.22%	0.925%
8	10.022	1258	1264	1276	rBV	269813	472162	14.24%	1.428%
9	10.393	1318	1327	1334	rBV	823445	1440705	43.44%	4.356%
10	10.534	1343	1351	1363	rBV	244479	480913	14.50%	1.454%
11	12.287	1644	1649	1657	rVB	19010	34553	1.04%	0.104%
12	13.581	1864	1869	1874	rBV2	21678	40616	1.22%	0.123%
13	13.675	1880	1885	1889	rBV	503520	722198	21.77%	2.184%
14	13.722	1889	1893	1904	rVB	583862	892142	26.90%	2.697%
15	13.957	1926	1933	1944	rBV	595619	984357	29.68%	2.976%
16	14.263	1976	1985	1993	rBV2	1126579	1898298	57.23%	5.740%
17	14.328	1993	1996	2004	rVB	38499	62173	1.87%	0.188%
18	14.492	2017	2024	2033	rBV4	79153	162415	4.90%	0.491%
19	14.669	2049	2054	2059	rVB6	21599	38313	1.16%	0.116%
20	14.886	2084	2091	2096	rBV6	13497	37204	1.12%	0.112%
21	15.057	2114	2120	2129	rBV5	18128	52836	1.59%	0.160%
22	15.263	2144	2155	2161	rBV	846476	1277634	38.52%	3.863%
23	15.316	2161	2164	2172	rVB3	27327	44762	1.35%	0.135%
24	15.398	2173	2178	2188	rVV3	77827	145061	4.37%	0.439%
25	15.533	2197	2201	2207	rVB2	34112	51287	1.55%	0.155%
26	16.016	2275	2283	2289	rBV2	68286	144906	4.37%	0.438%
27	16.316	2329	2334	2339	rBV7	15816	37799	1.14%	0.114%
28	16.786	2410	2414	2418	rBV2	24526	39979	1.21%	0.121%
29	16.833	2418	2422	2431	rVB3	59553	104130	3.14%	0.315%
30	17.016	2447	2453	2458	rBV	1558269	2314766	69.79%	6.999%
31	17.057	2458	2460	2464	rVV	146397	173166	5.22%	0.524%
32	17.116	2464	2470	2481	rVB	912278	1504294	45.35%	4.548%
33	17.433	2519	2524	2529	rBV8	21316	39074	1.18%	0.118%
34	17.522	2535	2539	2546	rVB4	24907	45150	1.36%	0.137%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
 Data File : BM006526.D
 Acq On : 19 Jul 2016 17:21
 Operator : UM/SJ
 Sample : H4029-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

35	17.598	2546	2552	2562	rVB6	15811	43894	1.32%	0.133%
36	17.886	2597	2601	2607	rBV	46005	73696	2.22%	0.223%
37	17.939	2607	2610	2615	rVB	40235	52359	1.58%	0.158%
38	18.022	2621	2624	2629	rVB2	25358	35692	1.08%	0.108%
39	18.086	2629	2635	2639	rVV3	82931	175619	5.29%	0.531%
40	18.122	2639	2641	2647	rVB	44537	57916	1.75%	0.175%
41	18.398	2684	2688	2693	rVB	36731	49658	1.50%	0.150%
42	18.816	2754	2759	2764	rBV	58541	98185	2.96%	0.297%
43	19.080	2799	2804	2810	rVV	327982	453922	13.69%	1.372%
44	19.139	2810	2814	2819	rVB6	34787	53652	1.62%	0.162%
45	19.233	2825	2830	2834	rBV	52298	78304	2.36%	0.237%
46	19.416	2855	2861	2865	rBV	1223576	1906087	57.47%	5.763%
47	19.527	2875	2880	2884	rBV3	29705	52056	1.57%	0.157%
48	19.621	2891	2896	2901	rBV4	21309	45248	1.36%	0.137%
49	19.774	2917	2922	2930	rVB3	35062	71925	2.17%	0.217%
50	19.945	2947	2951	2955	rVB	103347	135924	4.10%	0.411%
51	20.045	2964	2968	2972	rVV	100031	119876	3.61%	0.362%
52	20.104	2974	2978	2982	rVB2	49051	66695	2.01%	0.202%
53	20.245	2998	3002	3005	rBV	36435	47585	1.43%	0.144%
54	20.286	3006	3009	3014	rVB2	34433	53600	1.62%	0.162%
55	20.463	3036	3039	3043	rBV4	29072	38995	1.18%	0.118%
56	20.863	3104	3107	3110	rBV	31541	37249	1.12%	0.113%
57	20.898	3111	3113	3116	rVB	34833	35700	1.08%	0.108%
58	21.133	3148	3153	3160	rBV	2517283	2792326	84.19%	8.443%
59	21.215	3160	3167	3171	rVV	2216721	3316792	100.00%	10.029%
60	21.251	3171	3173	3181	rVB	254083	311087	9.38%	0.941%
61	21.368	3190	3193	3198	rBV2	51927	73945	2.23%	0.224%
62	21.968	3292	3295	3304	rVB3	122663	229169	6.91%	0.693%
63	22.757	3423	3429	3434	rBV2	174851	465497	14.03%	1.407%
64	23.221	3504	3508	3511	rBV	92879	160048	4.83%	0.484%
65	23.274	3511	3517	3522	rBV2	841130	1631394	49.19%	4.933%
66	23.409	3533	3540	3556	rVB	1482580	3059384	92.24%	9.250%
67	23.909	3622	3625	3636	rVB2	107679	222926	6.72%	0.674%
68	24.633	3744	3748	3757	rVB3	99964	215639	6.50%	0.652%
69	25.598	3907	3912	3923	rVB2	90993	256935	7.75%	0.777%


Sum of corrected areas: 33073411

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006526.D
Acq On : 19 Jul 2016 17:21
Operator : UM/SJ
Sample : H4029-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJA0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

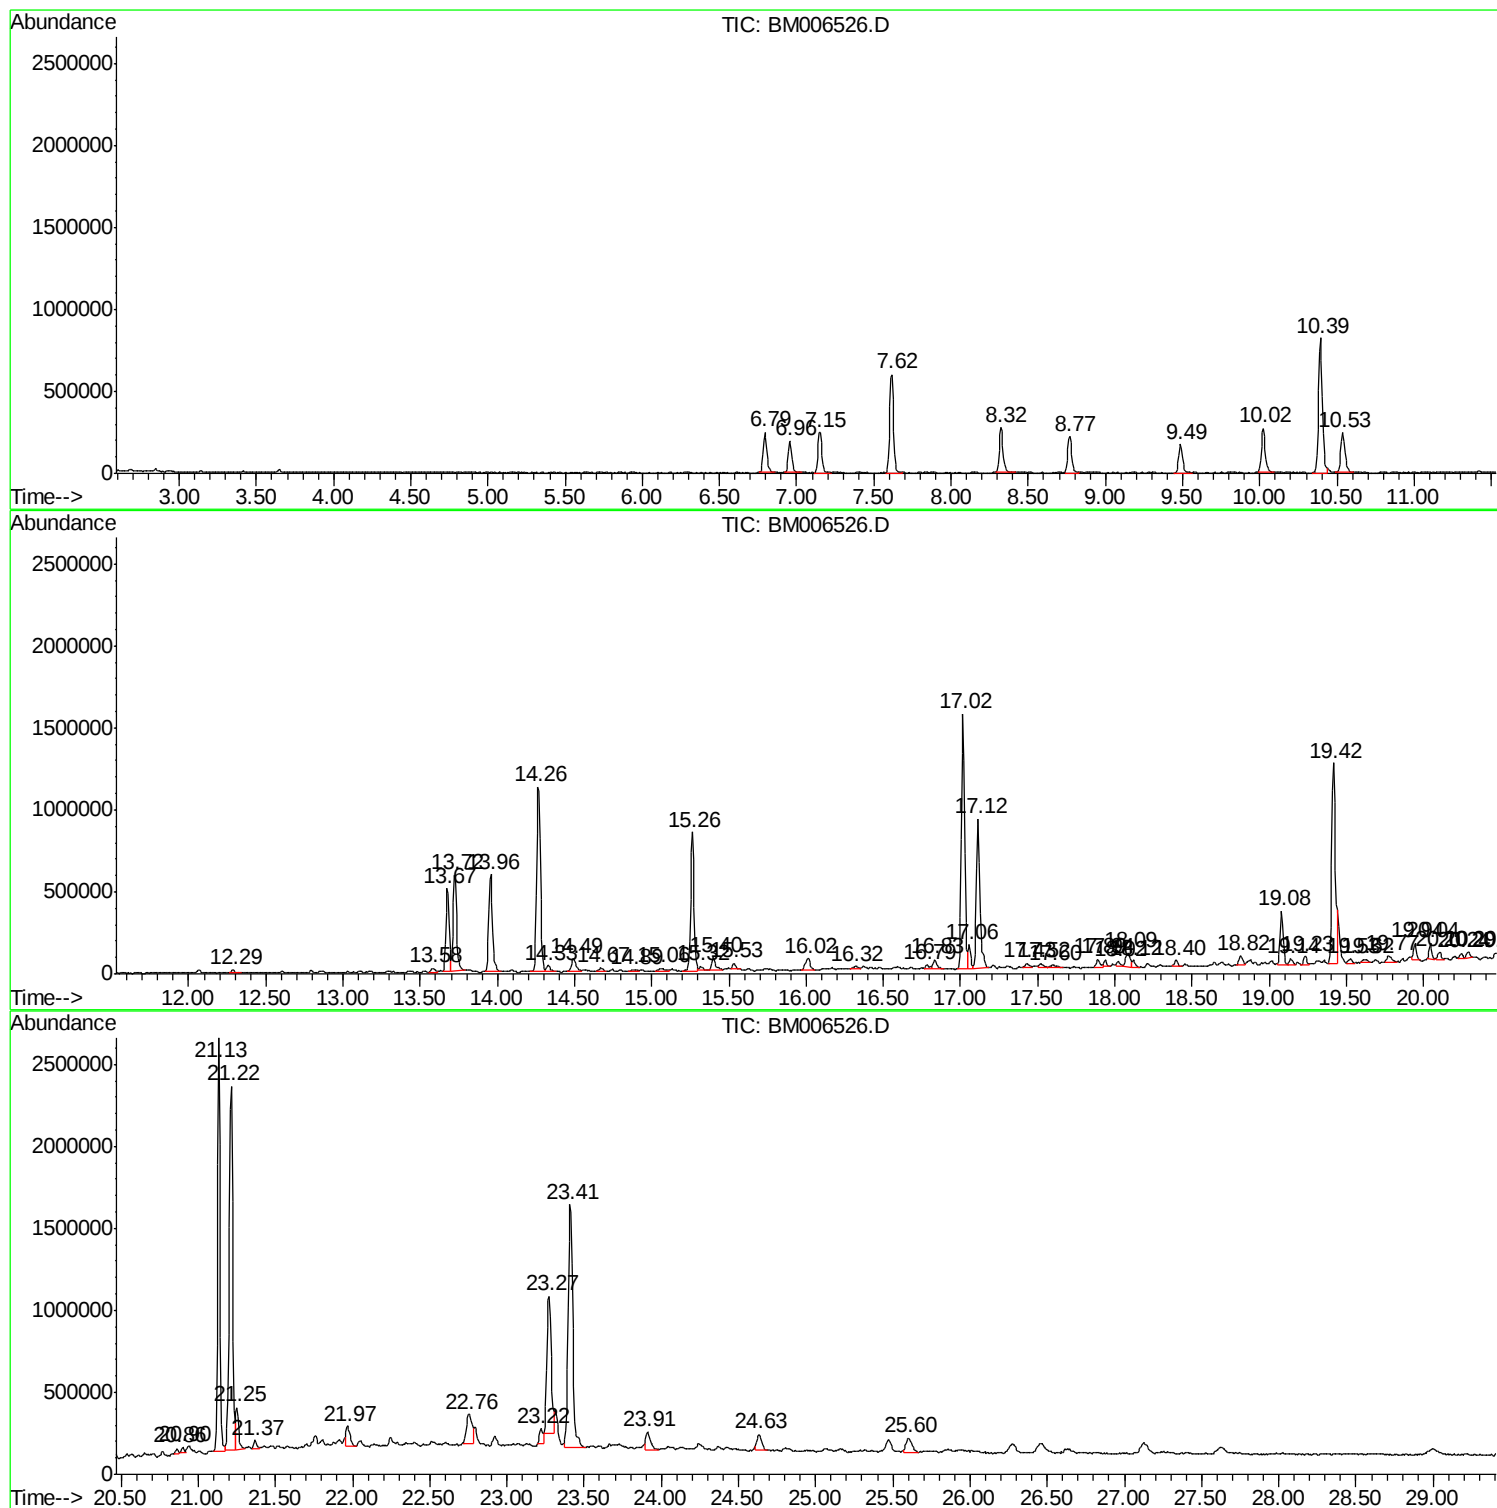

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006526.D
Acq On : 19 Jul 2016 17:21
Operator : UM/SJ
Sample : H4029-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJA0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006526.D
Acq On : 19 Jul 2016 17:21
Operator : UM/SJ
Sample : H4029-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJA0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc