

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
 Data File : BM006537.D
 Acq On : 20 Jul 2016 00:01
 Operator : UM/SJ
 Sample : H4029-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.792	709	715	730	rVB	547448	912141	23.28%	2.002%
2	6.957	733	743	756	rBV	425073	689071	17.59%	1.513%
3	7.145	769	775	785	rBV	549279	925290	23.62%	2.031%
4	7.616	847	855	864	rBV	700232	1176073	30.02%	2.582%
5	8.322	969	975	991	rVB	649520	1082520	27.63%	2.376%
6	8.769	1043	1051	1071	rBV	507615	879187	22.44%	1.930%
7	9.486	1165	1173	1187	rBV	398770	713213	18.20%	1.566%
8	10.022	1257	1264	1282	rVB	576472	1061485	27.09%	2.330%
9	10.392	1319	1327	1344	rBV	923116	1643623	41.95%	3.608%
10	10.533	1344	1351	1365	rBV	572559	1063780	27.15%	2.335%
11	13.674	1879	1885	1890	rBV	995067	1478866	37.74%	3.246%
12	13.721	1890	1893	1908	rVB	345901	525830	13.42%	1.154%
13	13.957	1926	1933	1951	rVB	1144339	1896355	48.40%	4.163%
14	14.262	1979	1985	1993	rBV2	1240553	2013461	51.39%	4.420%
15	14.486	2015	2023	2043	rBV	373418	714837	18.24%	1.569%
16	15.262	2146	2155	2163	rBV	1504434	2258506	57.64%	4.958%
17	15.398	2172	2178	2191	rBV	368444	587175	14.99%	1.289%
18	15.992	2274	2279	2286	rBV3	30705	63777	1.63%	0.140%
19	17.015	2446	2453	2458	rBV	1644937	2438960	62.25%	5.354%
20	17.056	2458	2460	2464	rVV	74214	91424	2.33%	0.201%
21	17.109	2464	2469	2481	rVB2	1600144	2580639	65.87%	5.665%
22	17.892	2597	2602	2606	rBV3	30477	47572	1.21%	0.104%
23	17.939	2606	2610	2615	rVB	27423	41865	1.07%	0.092%
24	18.086	2629	2635	2639	rVV3	72731	133433	3.41%	0.293%
25	18.815	2753	2759	2764	rBV2	47318	87001	2.22%	0.191%
26	18.880	2764	2770	2773	rVV6	25888	50565	1.29%	0.111%
27	19.080	2795	2804	2810	rBV	589934	810343	20.68%	1.779%
28	19.233	2825	2830	2835	rBV	63329	87734	2.24%	0.193%
29	19.415	2855	2861	2865	rBV	2263237	3409339	87.02%	7.484%
30	19.521	2875	2879	2885	rVB3	38513	66745	1.70%	0.147%
31	19.627	2892	2897	2902	rBV	36422	56101	1.43%	0.123%
32	19.768	2916	2921	2923	rBV3	53335	89347	2.28%	0.196%
33	19.909	2940	2945	2947	rBV4	46034	78258	2.00%	0.172%
34	19.944	2947	2951	2958	rVB2	182191	264235	6.74%	0.580%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006537.D
Acq On : 20 Jul 2016 00:01
Operator : UM/SJ
Sample : H4029-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION

35	20.044	2963	2968	2972	rVV	201514	252601	6.45%	0.554%
36	20.103	2972	2978	2981	rVV2	80040	127889	3.26%	0.281%
37	20.239	2998	3001	3006	rBV	47251	66298	1.69%	0.146%
38	20.286	3006	3009	3014	rVB2	51126	73395	1.87%	0.161%
39	20.650	3068	3071	3076	rBV3	37979	63164	1.61%	0.139%
40	20.856	3103	3106	3109	rBV	59302	73763	1.88%	0.162%
41	20.897	3110	3113	3116	rVV	68609	72846	1.86%	0.160%
42	20.933	3116	3119	3129	rVB4	74709	143938	3.67%	0.316%
43	21.127	3149	3152	3156	rVB	83858	98772	2.52%	0.217%
44	21.209	3159	3166	3170	rVV2	2527677	3918053	100.00%	8.600%
45	21.250	3170	3173	3183	rVB	421189	590609	15.07%	1.296%
46	21.368	3189	3193	3199	rBV	98614	153196	3.91%	0.336%
47	21.521	3215	3219	3224	rBV3	37986	66587	1.70%	0.146%
48	21.756	3253	3259	3263	rBV	104296	175926	4.49%	0.386%
49	21.909	3282	3285	3288	rVB2	46506	54148	1.38%	0.119%
50	21.944	3289	3291	3294	rVV2	61133	85855	2.19%	0.188%
51	21.980	3295	3297	3303	rVB2	95787	131081	3.35%	0.288%
52	22.244	3338	3342	3346	rBV5	57290	96063	2.45%	0.211%
53	22.750	3422	3428	3434	rBV	403309	1011834	25.82%	2.221%
54	22.921	3453	3457	3463	rVB2	117347	185963	4.75%	0.408%
55	23.221	3503	3508	3511	rBV	230566	409957	10.46%	0.900%
56	23.268	3511	3516	3521	rVV2	1637220	3099146	79.10%	6.803%
57	23.309	3521	3523	3530	rVB	422191	645097	16.46%	1.416%
58	23.409	3533	3540	3546	rBV	1659289	3134253	80.00%	6.880%
59	25.603	3906	3913	3921	rVB3	180410	490165	12.51%	1.076%
60	26.273	4020	4027	4039	rVB2	102487	317323	8.10%	0.697%


Sum of corrected areas: 45556673

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006537.D
Acq On : 20 Jul 2016 00:01
Operator : UM/SJ
Sample : H4029-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

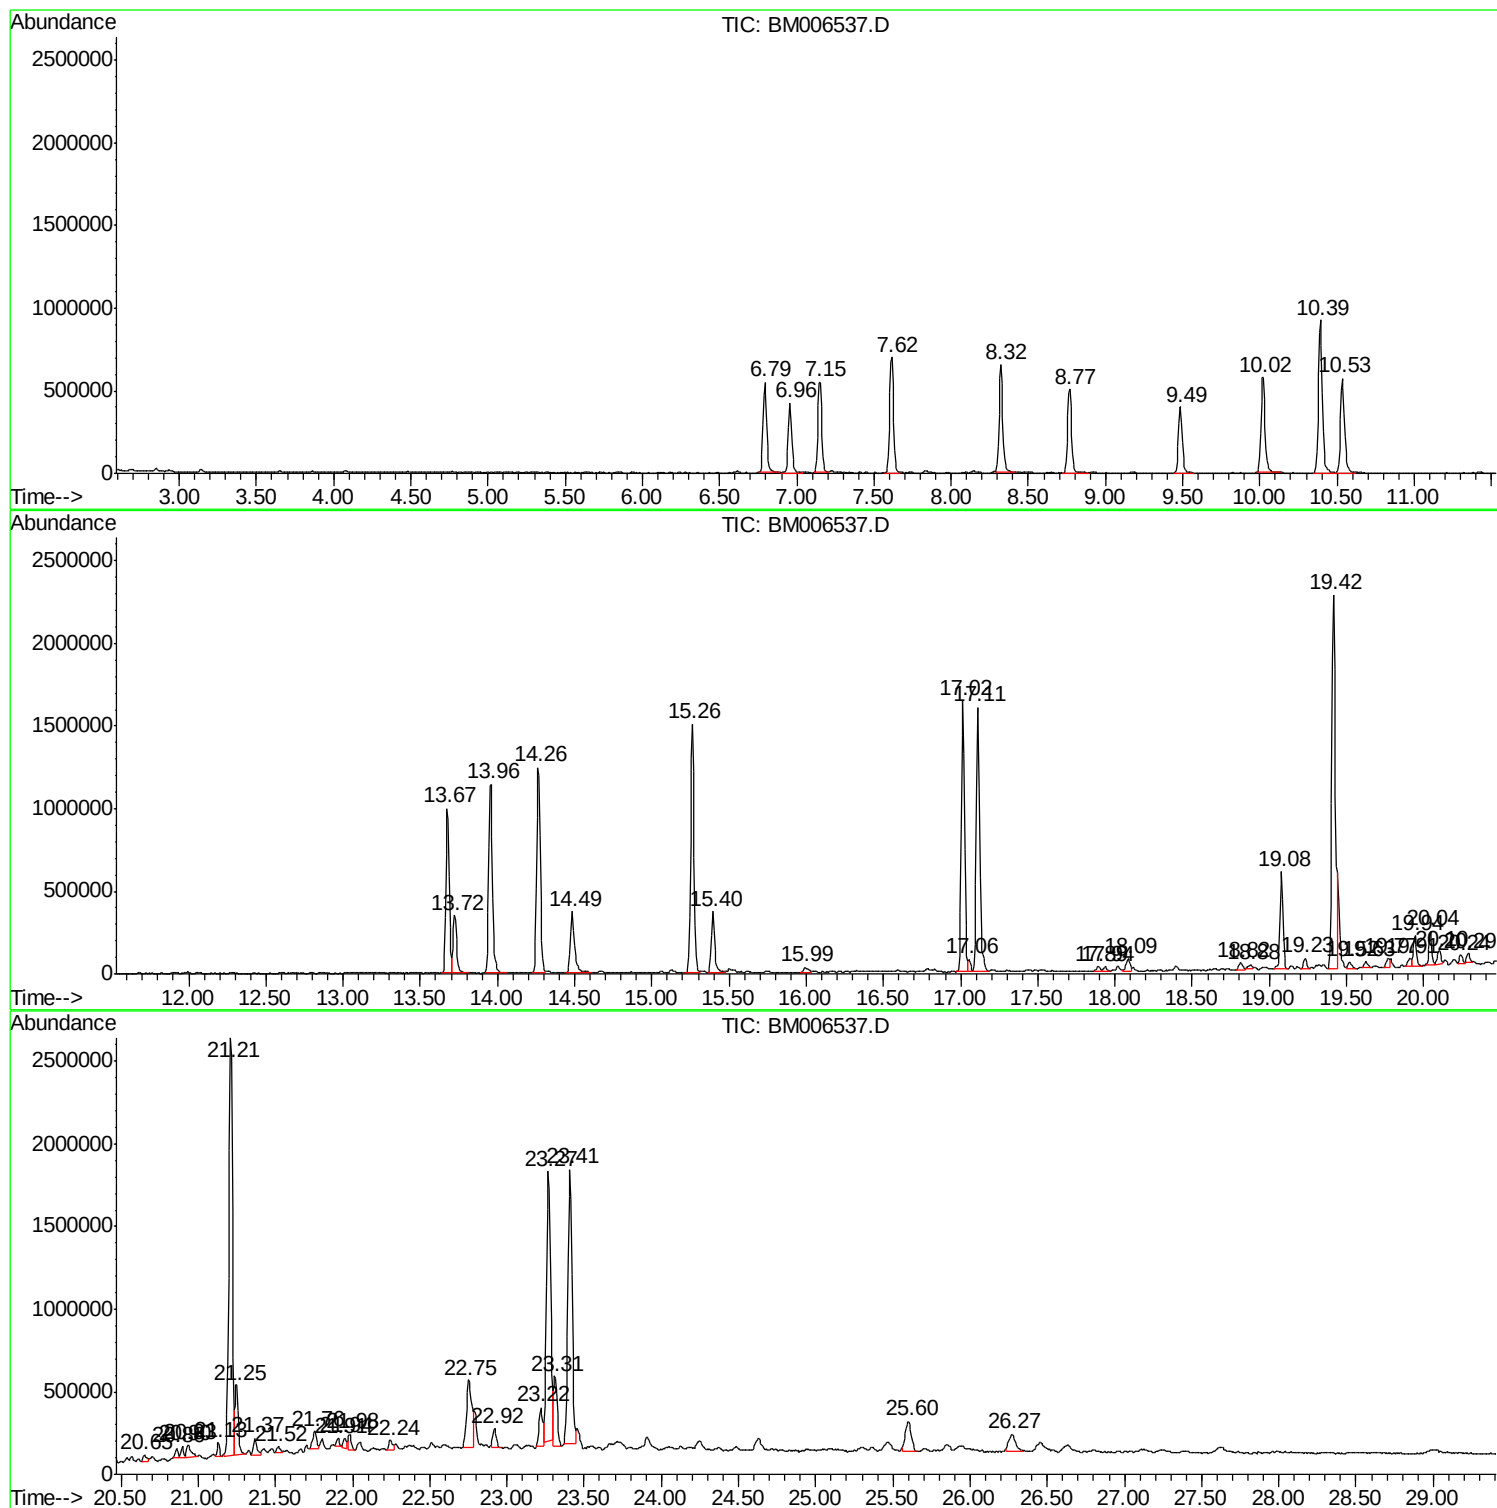

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006537.D
Acq On : 20 Jul 2016 00:01
Operator : UM/SJ
Sample : H4029-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006537.D
Acq On : 20 Jul 2016 00:01
Operator : UM/SJ
Sample : H4029-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc