

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
 Data File : BM006541.D
 Acq On : 20 Jul 2016 03:02
 Operator : UM/SJ
 Sample : H4029-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	729	rBV	542802	889170	23.35%	2.081%
2	6.951	736	742	755	rBV	405764	650202	17.07%	1.522%
3	7.145	769	775	792	rBV	537810	888646	23.33%	2.080%
4	7.610	847	854	865	rBV	716232	1201016	31.54%	2.811%
5	8.322	968	975	989	rBV	646667	1102637	28.95%	2.581%
6	8.769	1043	1051	1066	rBV	496207	873105	22.93%	2.043%
7	9.486	1166	1173	1190	rVB	410653	726142	19.07%	1.699%
8	10.016	1257	1263	1277	rBV	594773	1087190	28.55%	2.544%
9	10.392	1319	1327	1340	rBV	963163	1729358	45.41%	4.047%
10	10.533	1344	1351	1368	rBV	613422	1117251	29.34%	2.615%
11	13.674	1879	1885	1890	rBV	1161941	1717203	45.09%	4.019%
12	13.722	1890	1893	1909	rVB	470194	693494	18.21%	1.623%
13	13.951	1926	1932	1947	rBV	1240744	1988235	52.21%	4.653%
14	14.263	1978	1985	1999	rVB2	1392331	2264988	59.47%	5.301%
15	14.480	2016	2022	2038	rBV	496250	876027	23.00%	2.050%
16	15.263	2148	2155	2167	rBV	1686305	2559986	67.22%	5.991%
17	15.392	2172	2177	2190	rBV	499081	754543	19.81%	1.766%
18	15.992	2273	2279	2286	rBV2	27291	55387	1.45%	0.130%
19	16.780	2408	2413	2419	rBV3	26088	44926	1.18%	0.105%
20	17.015	2446	2453	2459	rBV	1819937	2770160	72.74%	6.483%
21	17.110	2463	2469	2482	rVB	1890903	2869341	75.34%	6.715%
22	19.080	2800	2804	2810	rVB	94294	131202	3.45%	0.307%
23	19.303	2835	2842	2847	rBV	20865	38542	1.01%	0.090%
24	19.415	2854	2861	2875	rBV	2465344	3528093	92.64%	8.257%
25	20.933	3115	3119	3126	rBV6	47357	101234	2.66%	0.237%
26	21.127	3149	3152	3157	rBV	65817	76560	2.01%	0.179%
27	21.209	3160	3166	3172	rBV	2776072	3690544	96.91%	8.637%
28	22.239	3338	3341	3349	rBV3	45866	75024	1.97%	0.176%
29	22.739	3422	3426	3434	rBV3	85731	206327	5.42%	0.483%
30	23.268	3504	3516	3528	rBV2	1878165	3808411	100.00%	8.913%
31	23.409	3532	3540	3553	rVB	1912310	3589123	94.24%	8.400%
32	23.909	3620	3625	3633	rVB	108463	210136	5.52%	0.492%
33	24.627	3742	3747	3757	rVB2	105656	229726	6.03%	0.538%
34	25.468	3885	3890	3899	rVB3	74027	184322	4.84%	0.431%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006541.D
Acq On : 20 Jul 2016 03:02
Operator : UM/SJ
Sample : H4029-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION


Sum of corrected areas: 42728251

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006541.D
Acq On : 20 Jul 2016 03:02
Operator : UM/SJ
Sample : H4029-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

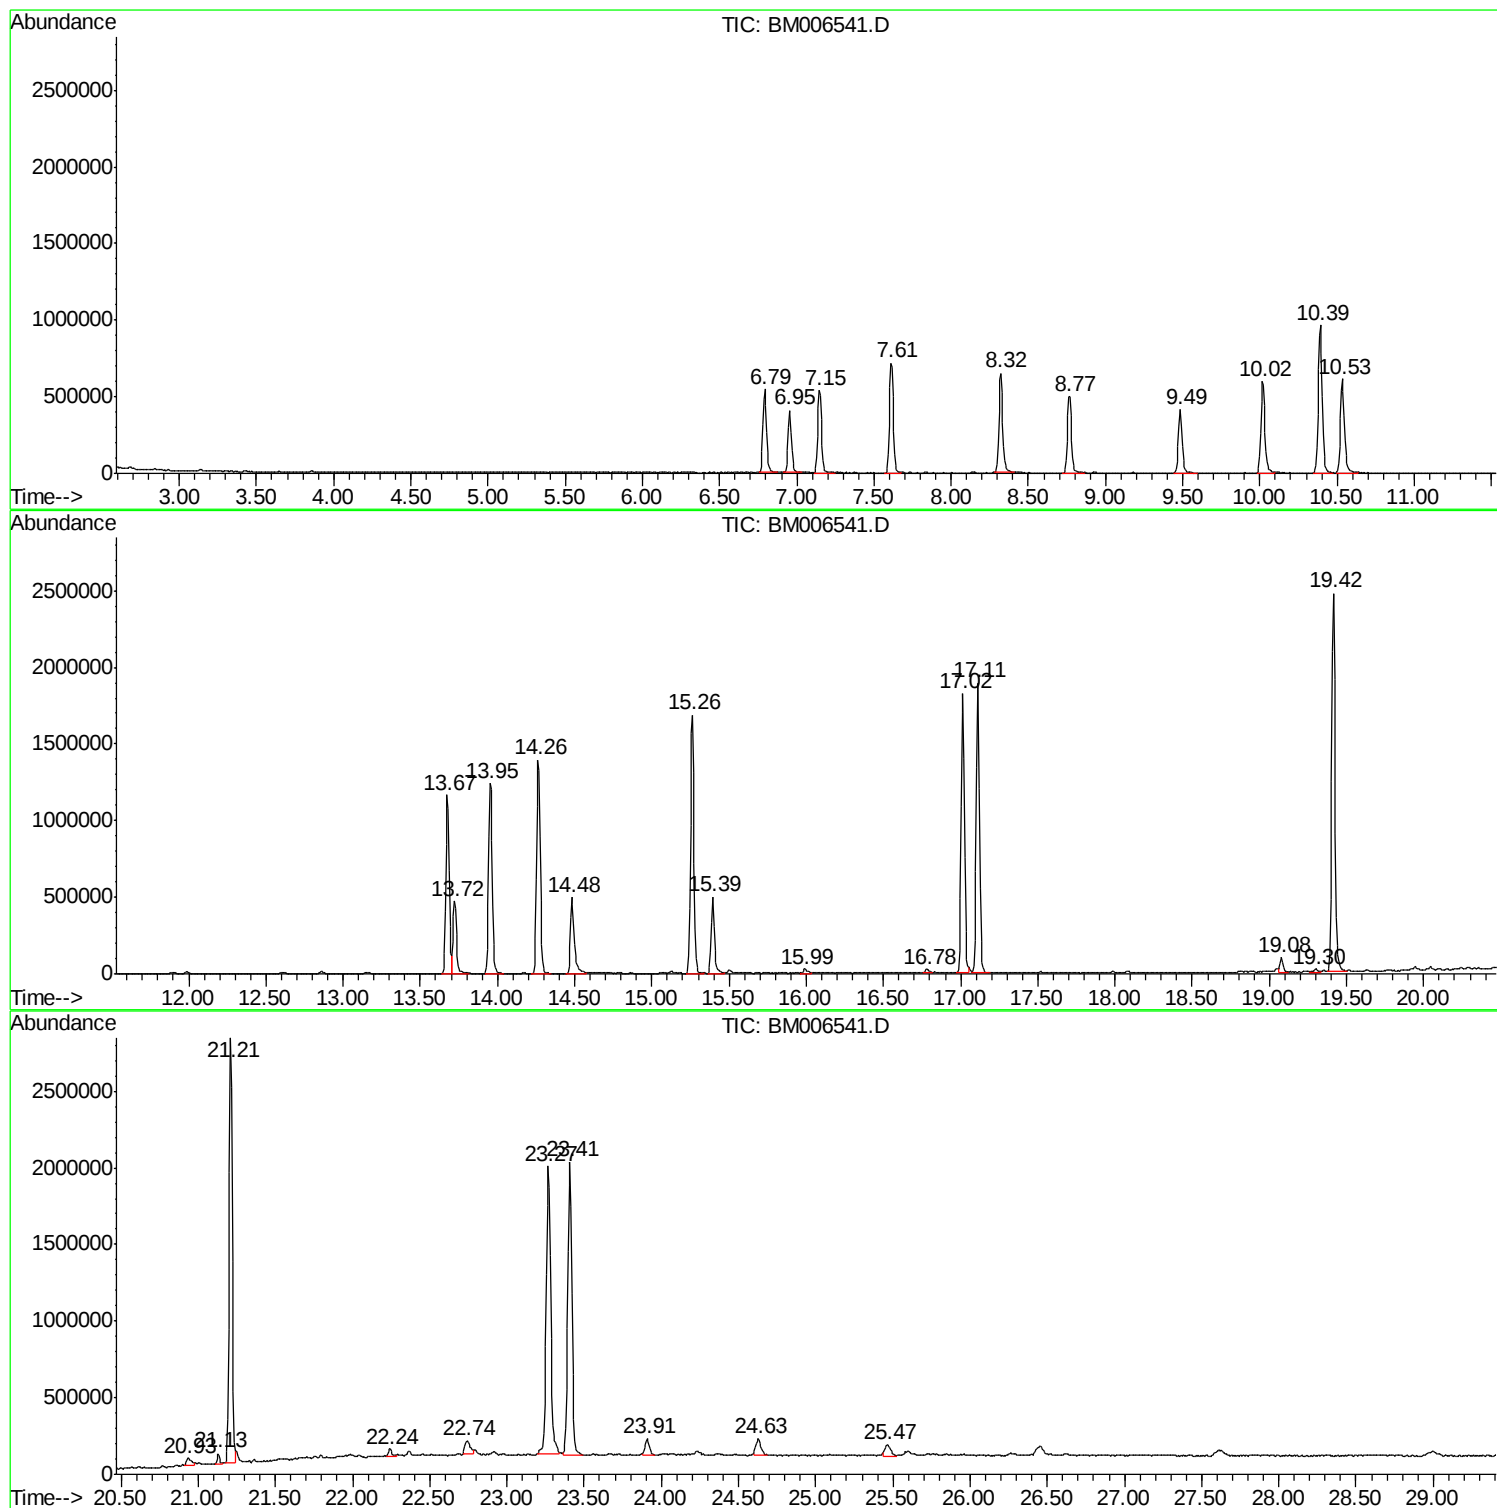

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006541.D
Acq On : 20 Jul 2016 03:02
Operator : UM/SJ
Sample : H4029-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071916\
Data File : BM006541.D
Acq On : 20 Jul 2016 03:02
Operator : UM/SJ
Sample : H4029-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJB4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc