


Data Path : Z:\HPCHEM1\BNA_M\Data\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 12 14:21:16 2017

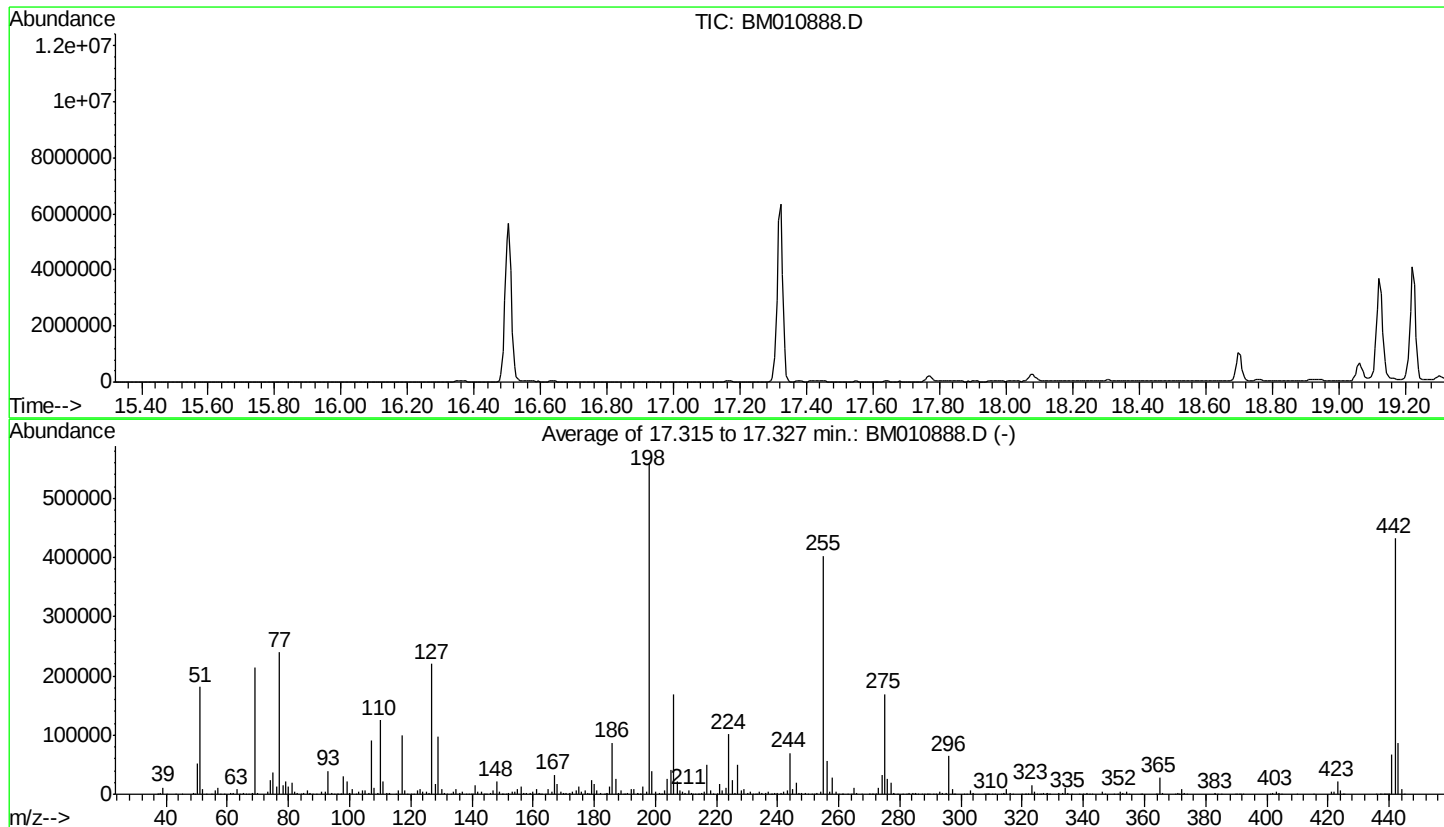

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	181586	PASS
68	69	0.00	2	1.4	3074	PASS
69	198	0.00	100	38.1	213674	PASS
70	69	0.00	2	0.7	1503	PASS
127	198	10	80	39.3	220352	PASS
197	198	0.00	2	0.7	3865	PASS
198	198	100	100	100.0	560128	PASS
199	198	5	9	7.0	39240	PASS
275	198	10	60	30.2	169045	PASS
365	198	1	100	5.0	27760	PASS
441	443	0.01	100	78.8	67960	PASS
442	198	50	100	77.1	432021	PASS
443	442	15	24	20.0	86194	PASS