
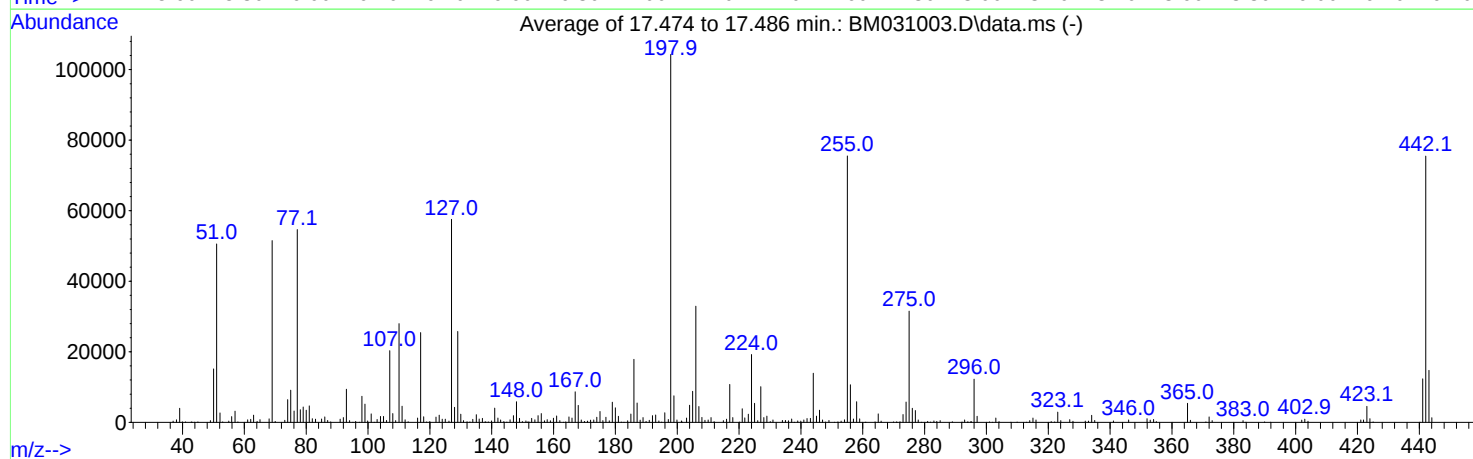


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071921\
 Data File : BM031003.D
 Acq On : 19 Jul 2021 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 19 18:48:56 2021

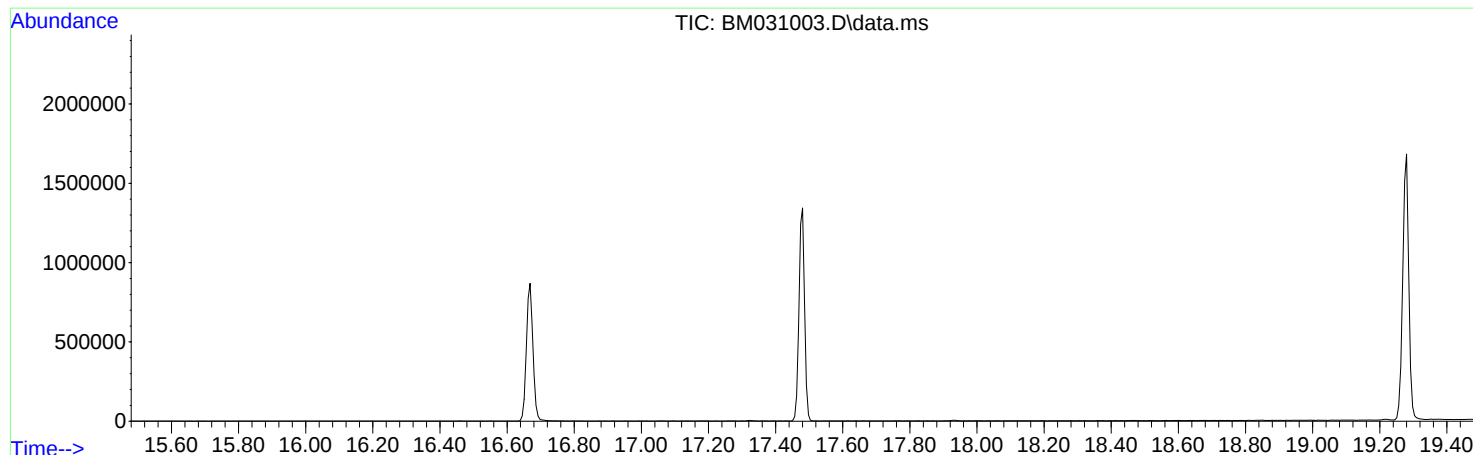




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	50563	PASS
68	69	0.00	2	1.9	1004	PASS
69	198	0.00	100	49.4	51525	PASS
70	69	0.00	2	0.6	291	PASS
127	198	10	80	55.2	57560	PASS
197	198	0.00	2	0.8	814	PASS
198	198	100	100	100.0	104283	PASS
199	198	5	9	7.2	7514	PASS
275	198	10	60	30.2	31525	PASS
365	198	1	100	5.2	5396	PASS
441	198	0.01	100	11.8	12324	PASS
442	442	50	100	100.0	75501	PASS
443	442	15	24	19.5	14735	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071921\
 Data File : BM031003.D
 Acq On : 19 Jul 2021 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 19 18:22:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 16:47:00 2021
 Response via : Initial Calibration

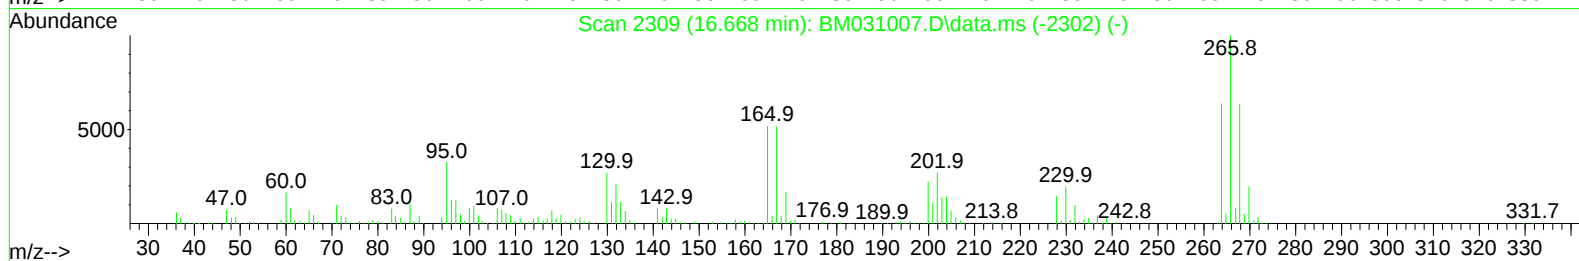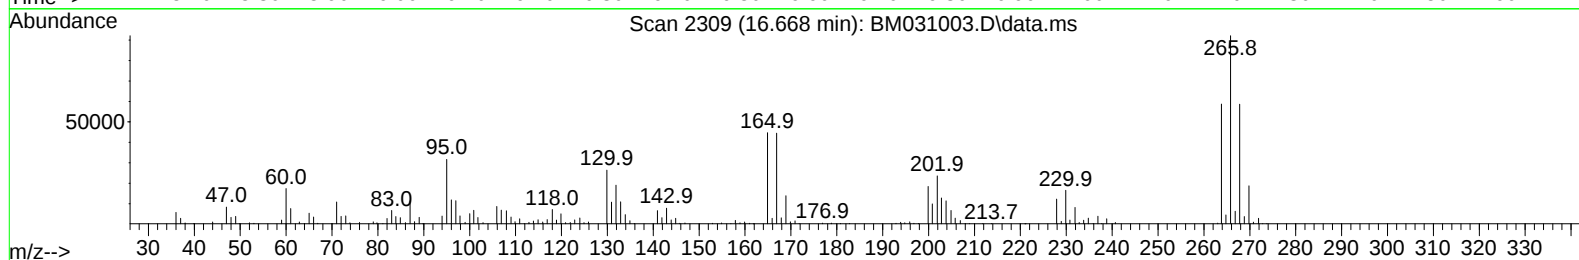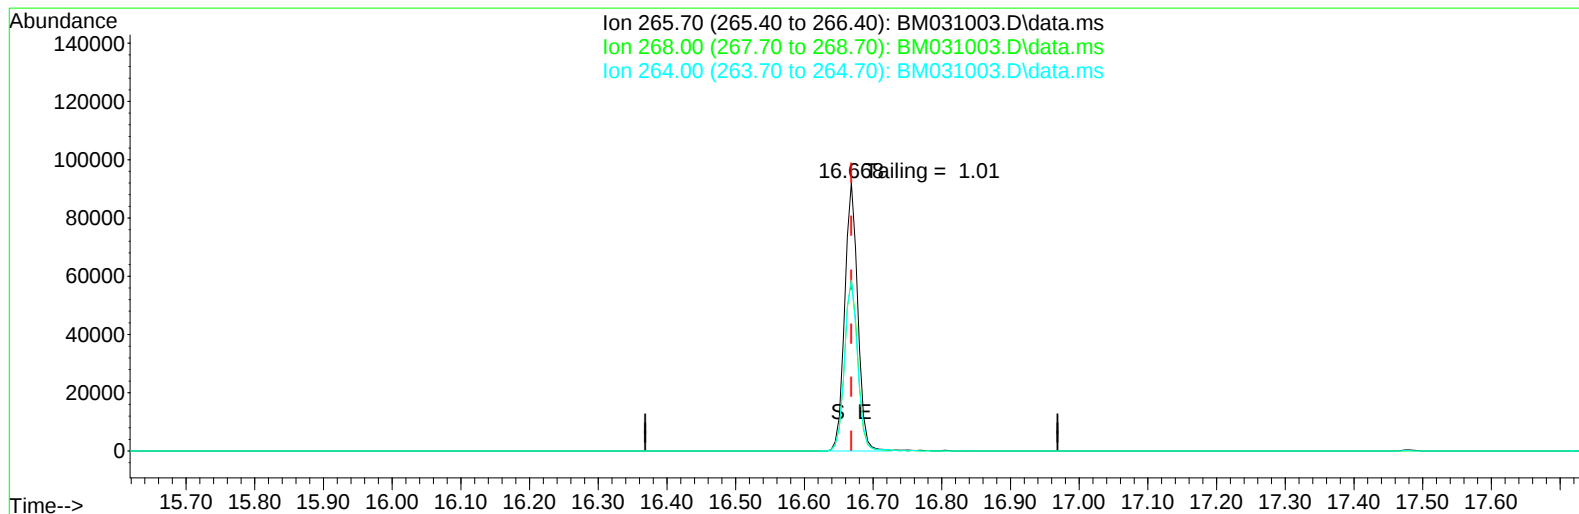

TIC: BM031003.D\data.ms

(70) Pentachlorophenol (C)

16.668min (+ 0.000) 0.00 ng




response 121462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.68
264.00	64.90	63.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071921\
Data File : BM031003.D
Acq On : 19 Jul 2021 13:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 19 18:22:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 16:47:00 2021
Response via : Initial Calibration

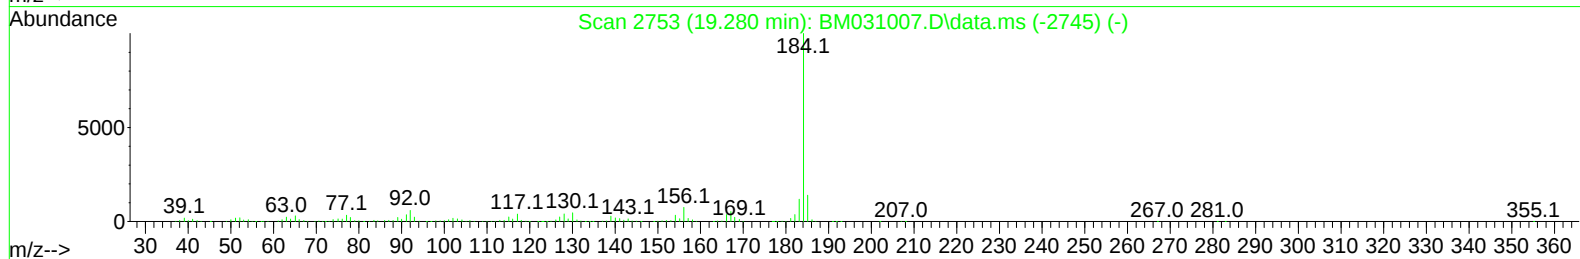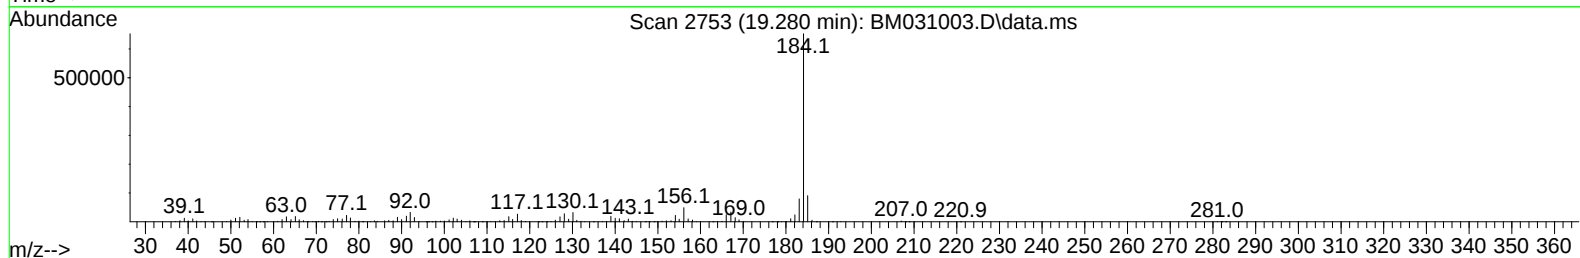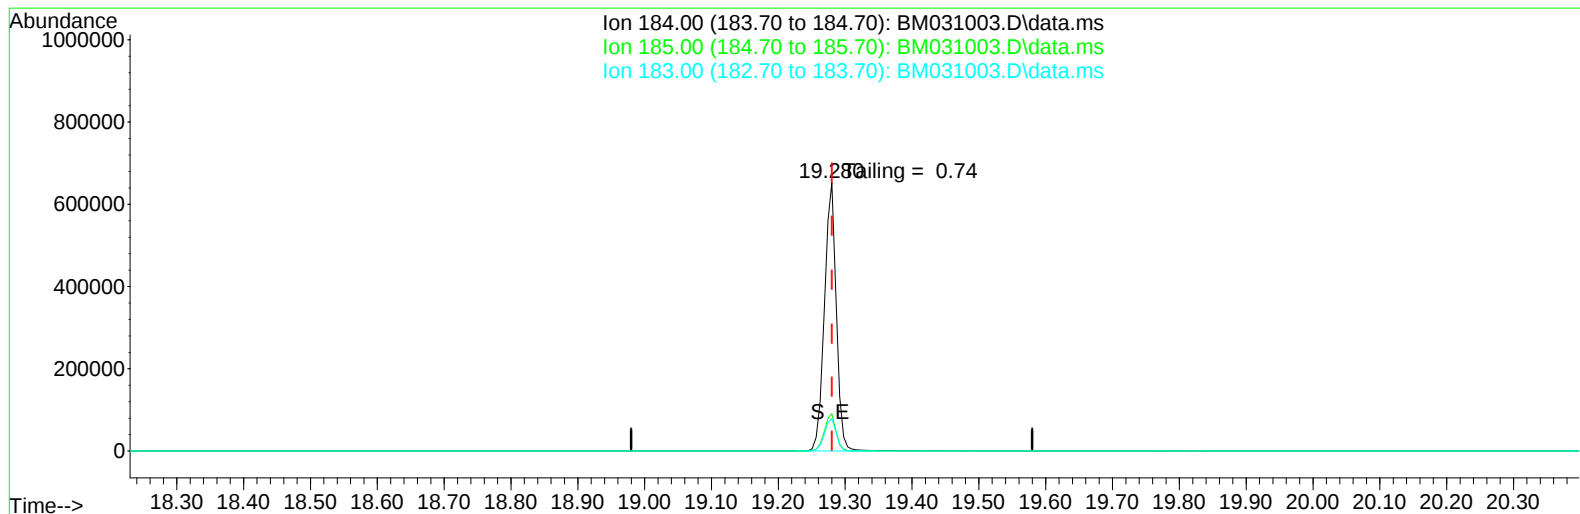

TIC: BM031003.D\data.ms

(77) Benzidine

19.280min (+ 0.000) 0.00 ng

response 805769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.91
183.00	12.30	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/19/2021	BNA_M	<u>BM031003.D</u>
Compound Name	Response	Retention Time
DDT	463767	20.51
DDD	922	20.07
DDE	529	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1451	465218	0.31

Instrument :
BNA_M
ClientSampleId :
DFTPP