
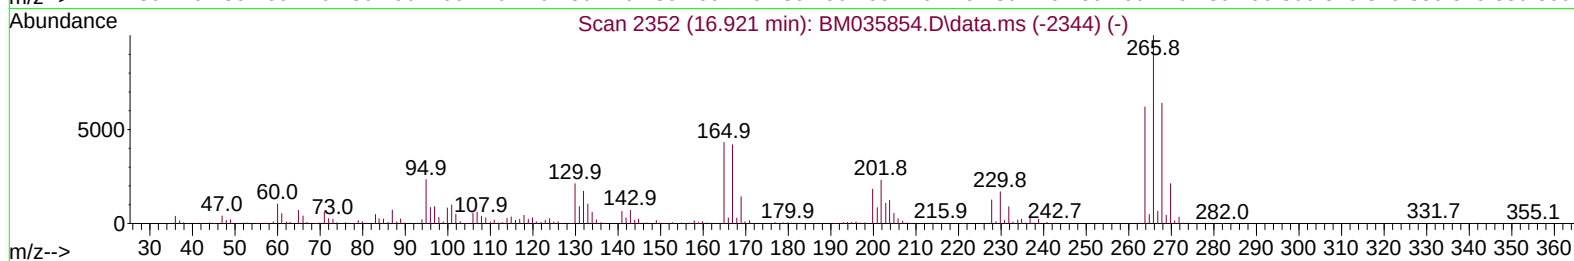
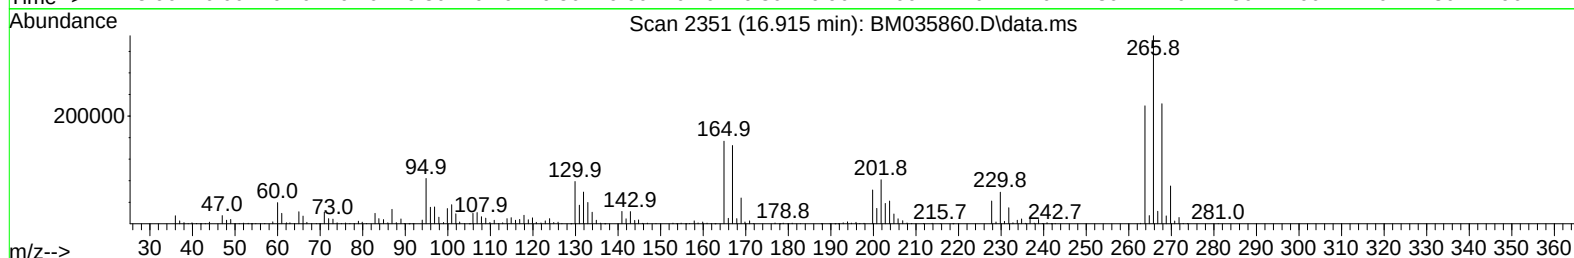


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
Data File : BM035860.D
Acq On : 19 Jul 2022 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:01:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 18 17:08:15 2022
Response via : Initial Calibration

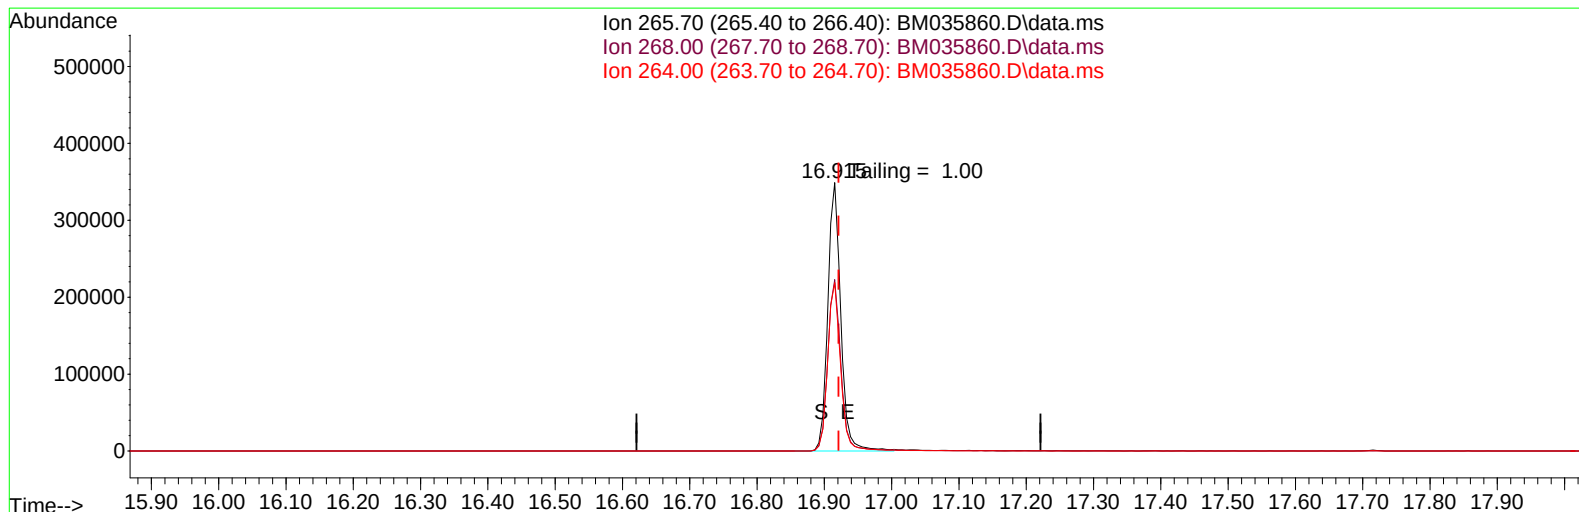

TIC: BM035860.D\data.ms

(70) Pentachlorophenol (C)




16.915min (-0.006) 0.00 ng

response 468356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.84
264.00	63.30	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
 Data File : BM035860.D
 Acq On : 19 Jul 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:01:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 18 17:08:15 2022
 Response via : Initial Calibration

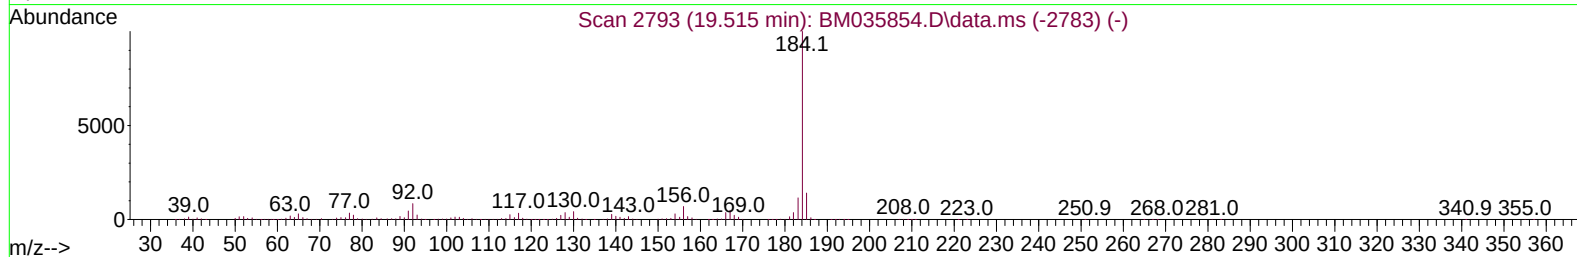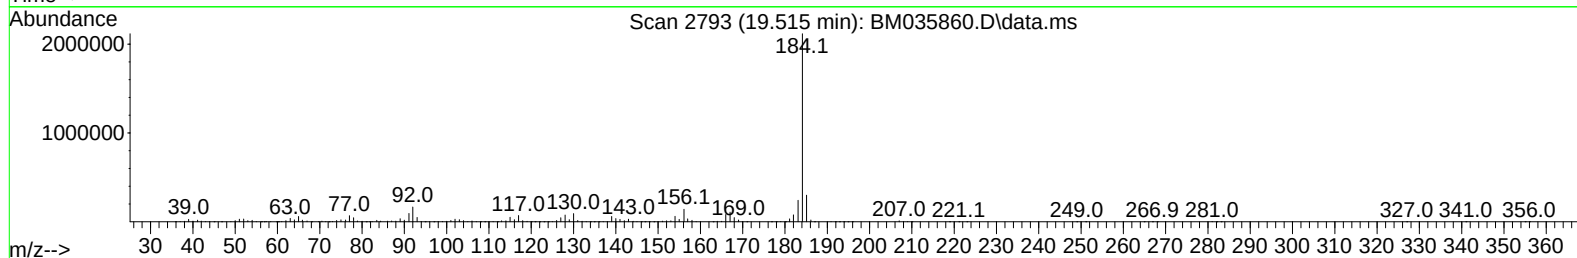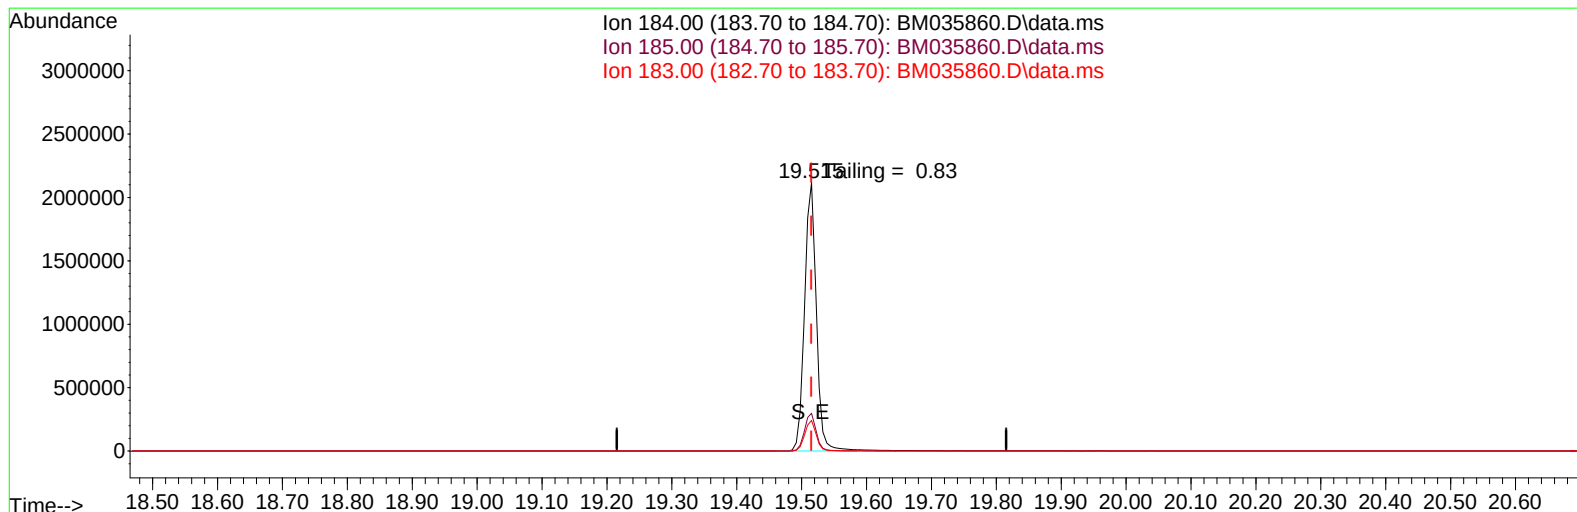

TIC: BM035860.D\data.ms

(77) Benzidine

19.515min (+ 0.000) 0.00 ng

response 2693514

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.90	11.43
0.00	0.00	0.00