

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
 Data File : BM035862.D
 Acq On : 19 Jul 2022 11:52
 Operator : CG/JU
 Sample : PB145921BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145921BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.045	159	163	169	rBV	108743	144170	1.20%	0.209%
2	5.457	397	403	422	rBV	6367088	9044208	75.27%	13.083%
3	7.069	669	677	686	rBV	5743286	9092866	75.67%	13.154%
4	7.898	811	818	828	rBV	1192857	1802916	15.00%	2.608%
5	9.063	1008	1016	1028	rBV	3424329	5594766	46.56%	8.093%
6	10.704	1288	1295	1304	rBV	1521788	2468263	20.54%	3.571%
7	13.163	1706	1713	1726	rBV	8564861	12015815	100.00%	17.382%
8	14.533	1937	1946	1955	rBV	2023896	2865432	23.85%	4.145%
9	16.015	2191	2198	2218	rBV	5077700	7049898	58.67%	10.198%
10	17.268	2405	2411	2421	rBV	2083470	2885349	24.01%	4.174%
11	19.892	2851	2857	2868	rBV	9921504	11786380	98.09%	17.050%
12	21.444	3116	3121	3128	rBV	1895484	2295082	19.10%	3.320%
13	23.821	3518	3525	3537	rVB2	1058669	2081752	17.33%	3.011%




Sum of corrected areas: 69126897

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
Data File : BM035862.D
Acq On : 19 Jul 2022 11:52
Operator : CG/JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

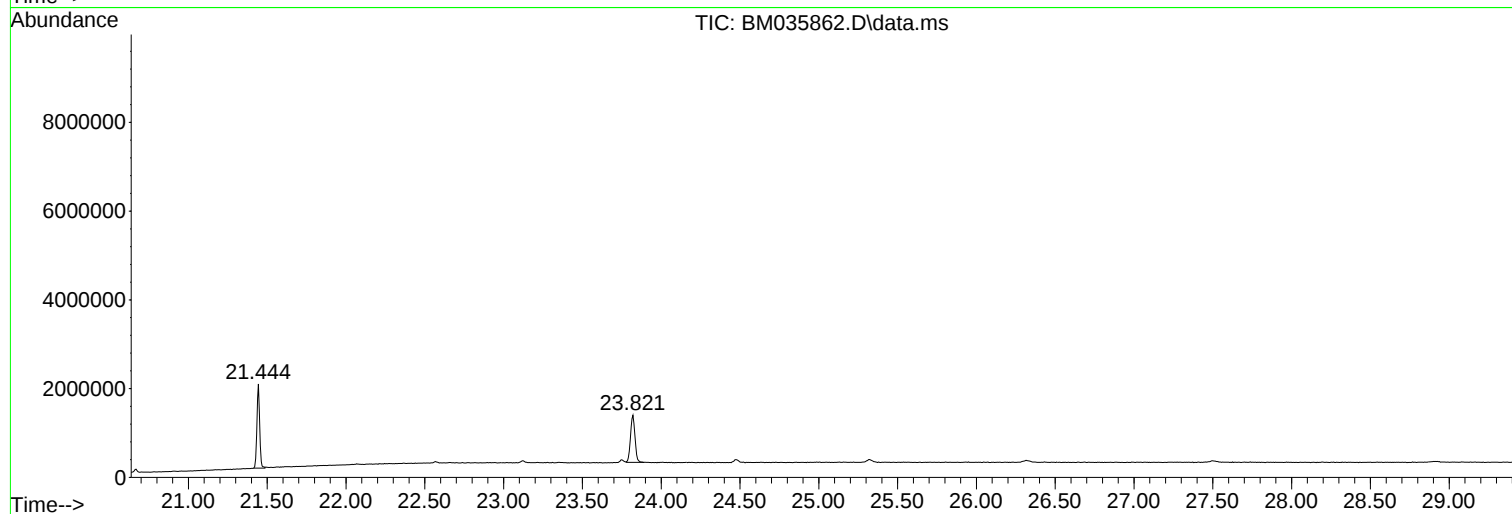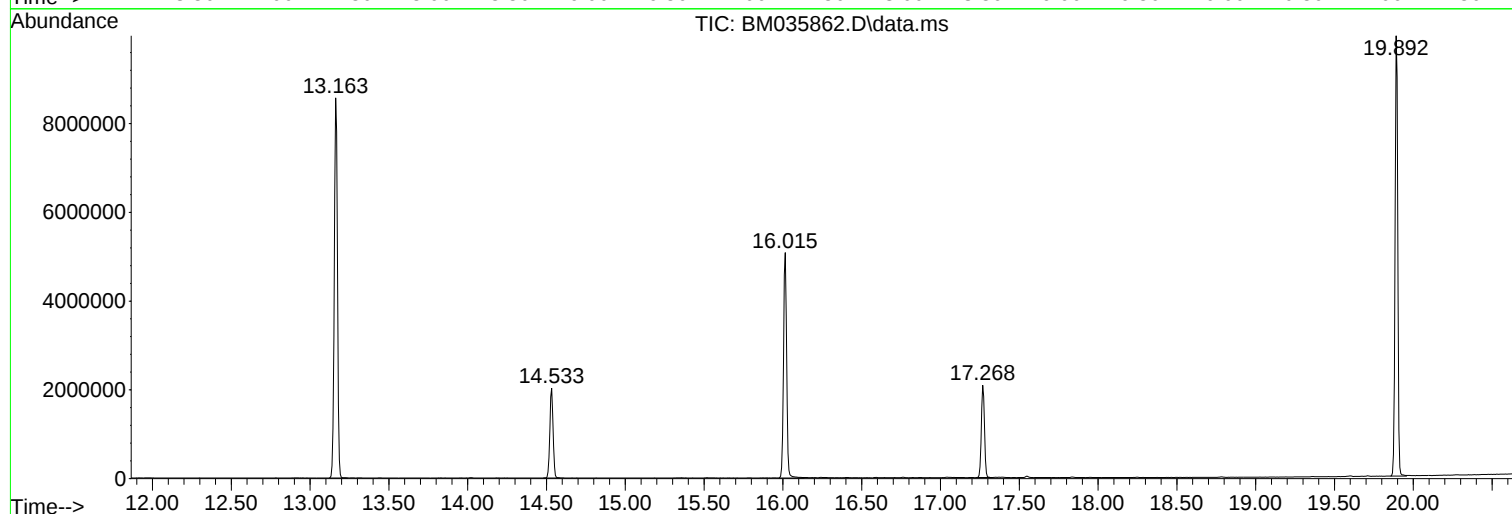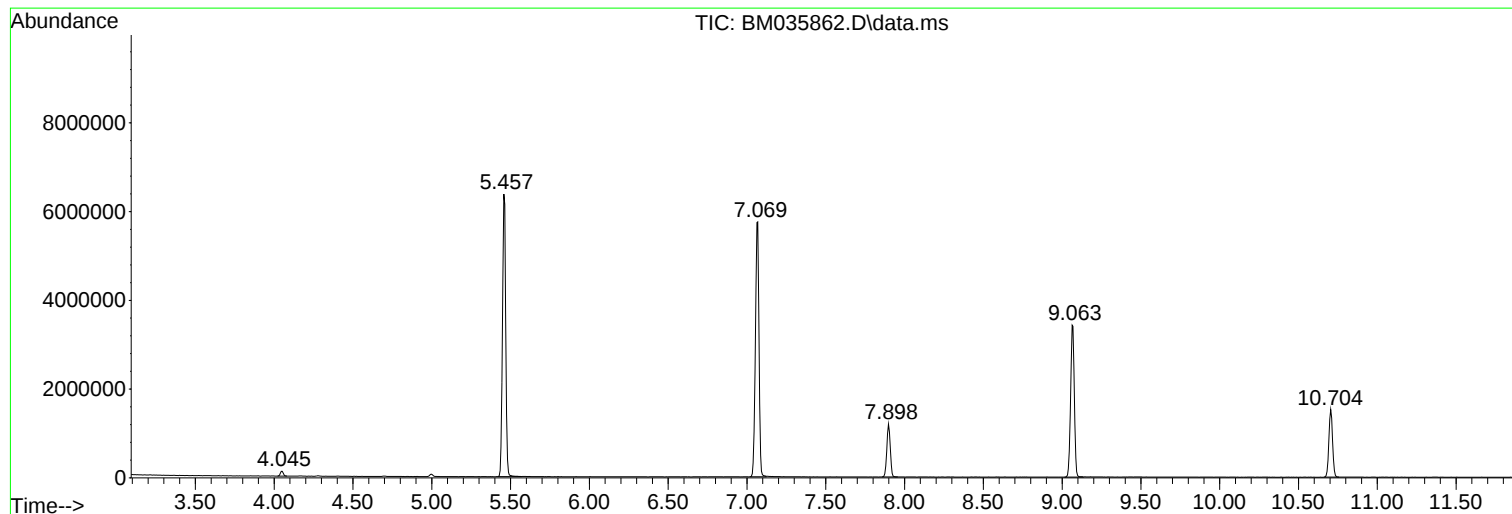

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
Data File : BM035862.D
Acq On : 19 Jul 2022 11:52
Operator : CG/JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
Data File : BM035862.D
Acq On : 19 Jul 2022 11:52
Operator : CG/JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------