
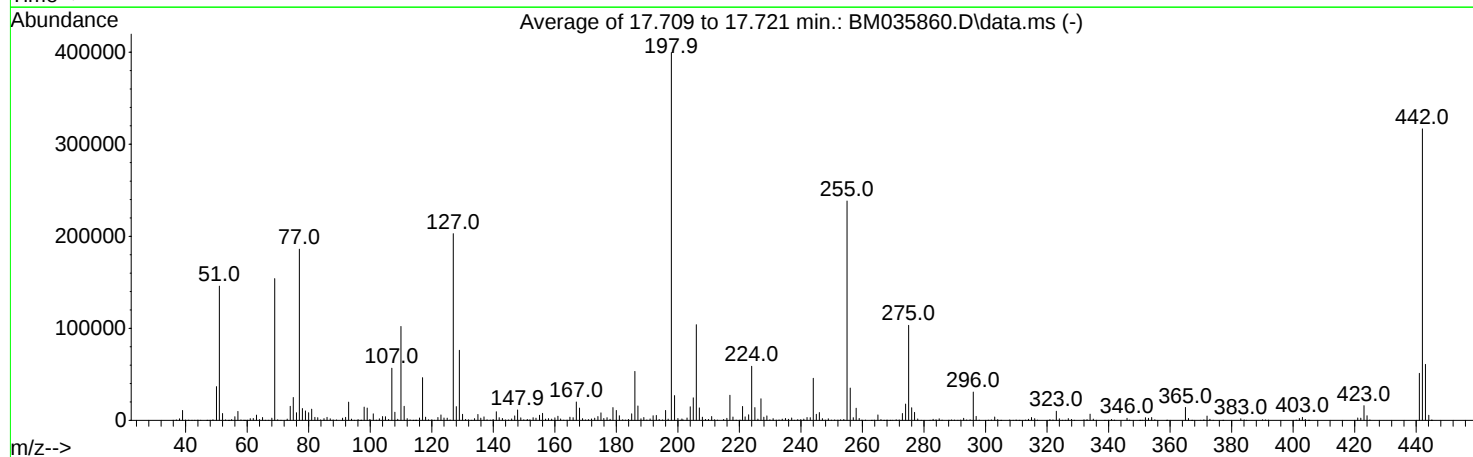


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
 Data File : BM035860.D
 Acq On : 19 Jul 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 18 17:08:15 2022

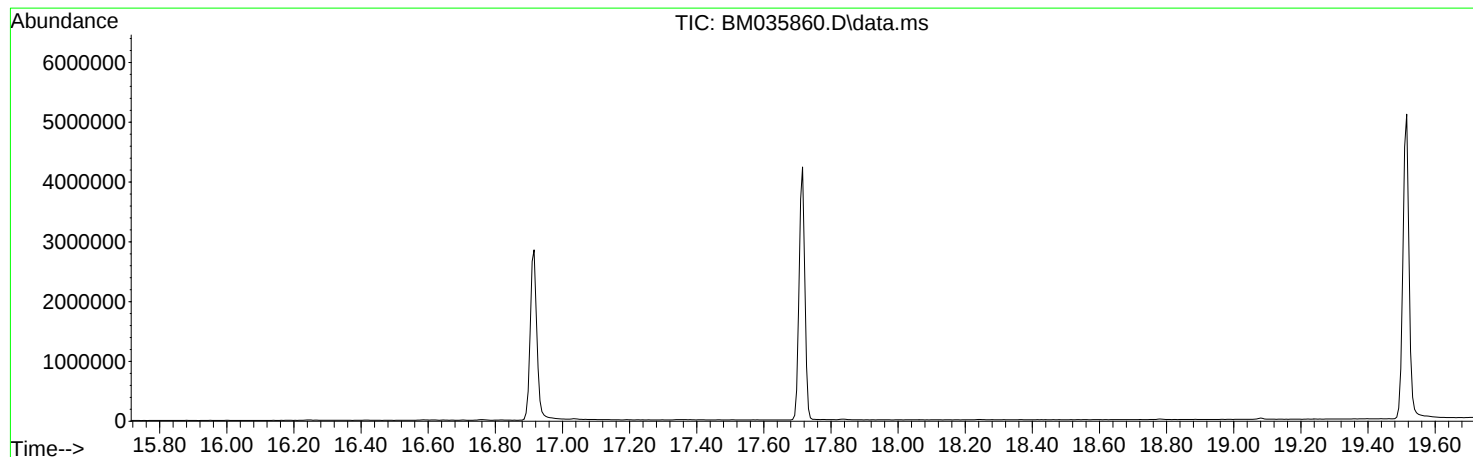




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	145913	PASS
68	69	0.00	2	1.6	2417	PASS
69	198	0.00	100	38.5	154070	PASS
70	69	0.00	2	0.5	722	PASS
127	198	10	80	50.8	202859	PASS
197	198	0.00	2	0.4	1452	PASS
198	198	100	100	100.0	399701	PASS
199	198	5	9	6.8	27021	PASS
275	198	10	60	25.8	103288	PASS
365	198	1	100	3.5	14016	PASS
441	198	0.01	100	12.8	51171	PASS
442	442	50	100	100.0	316693	PASS
443	442	15	24	19.2	60837	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
Data File : BM035860.D
Acq On : 19 Jul 2022 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 19 18:01:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 18 17:08:15 2022
Response via : Initial Calibration

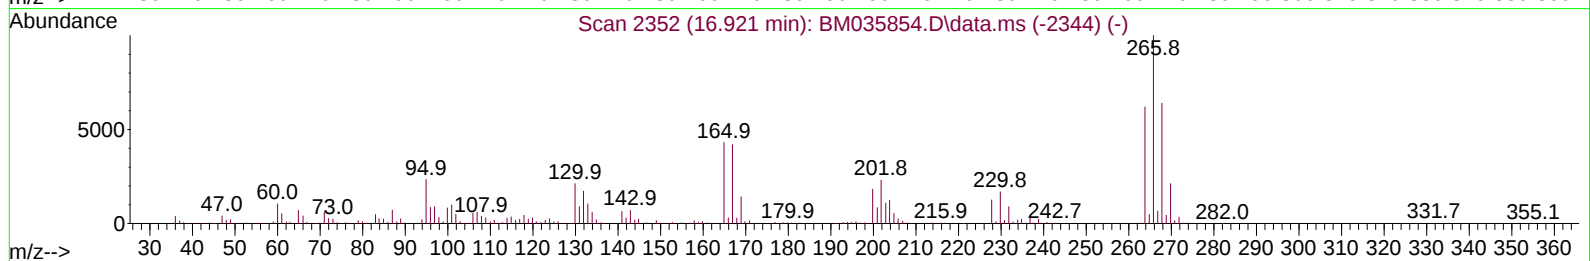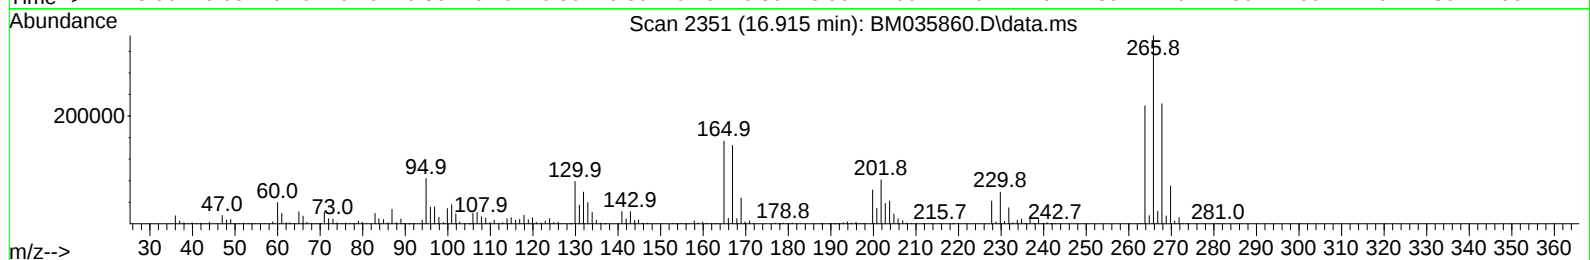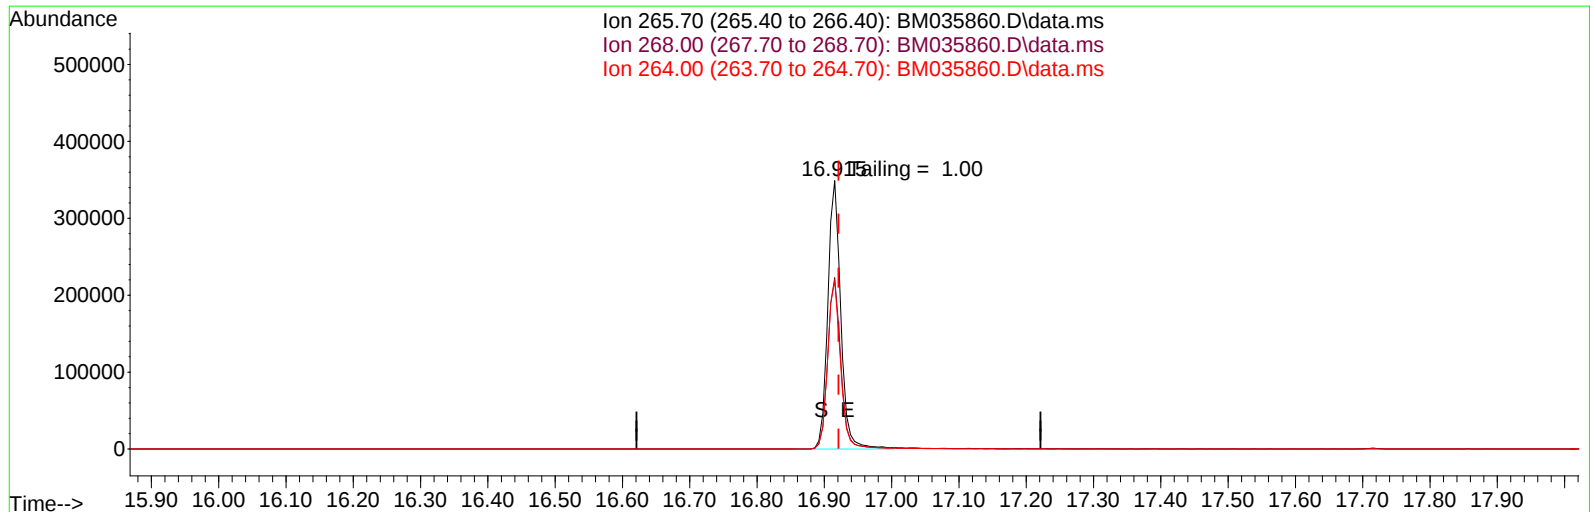

TIC: BM035860.D\data.ms

(70) Pentachlorophenol (C)

16.915min (-0.006) 0.00 ng




response 468356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.84
264.00	63.30	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071922\
 Data File : BM035860.D
 Acq On : 19 Jul 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 19 18:01:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 18 17:08:15 2022
 Response via : Initial Calibration

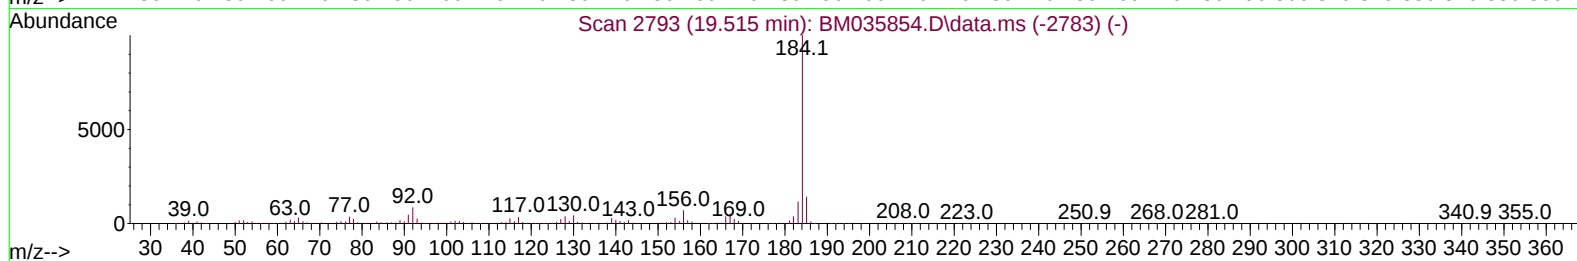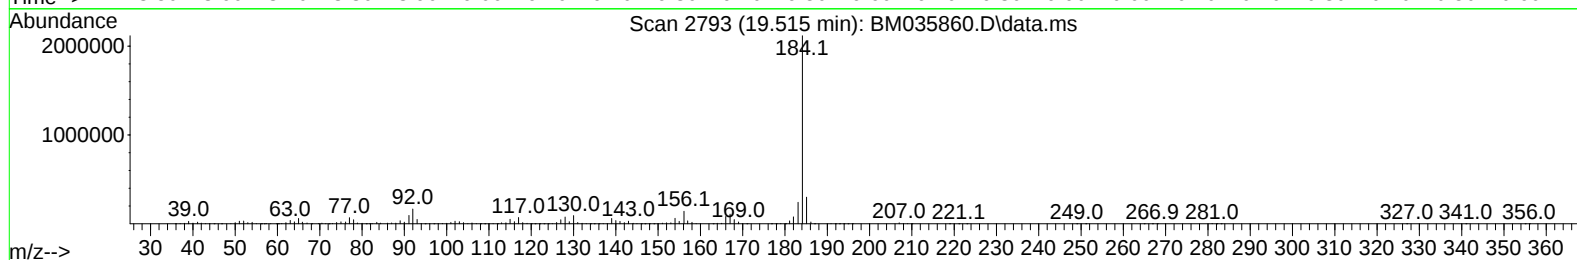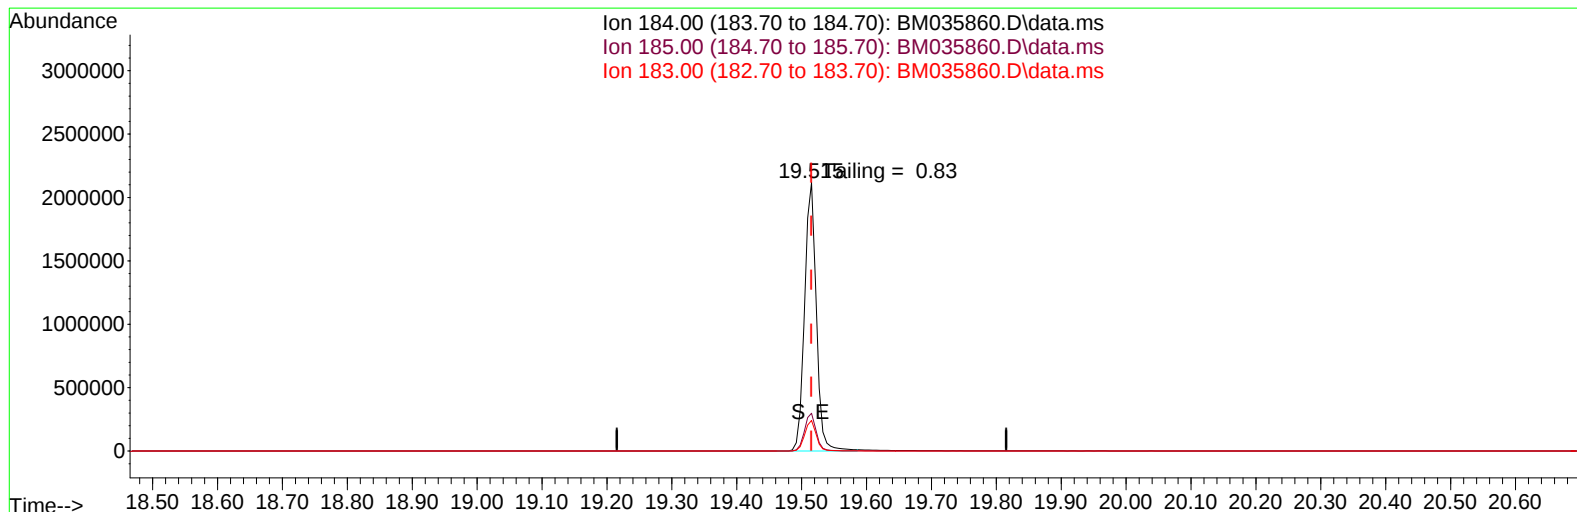

TIC: BM035860.D\data.ms

(77) Benzidine

19.515min (+ 0.000) 0.00 ng

response 2693514

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.90	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/19/2022	BNA_M	<u>BM035860.D</u>
Compound Name	Response	Retention Time
DDT	1276631	20.74
DDD	4883	20.3
DDE	557	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5440	1282071	0.42

Instrument :
BNA_M
ClientSampleId :
DFTPP