

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072015\
 Data File : BM001994.D
 Acq On : 21 Jul 2015 03:30
 Operator : TP/UM
 Sample : G3000-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02B9

Quant Time: Jul 21 04:05:54 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 21 01:37:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	111861	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	460942	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	267391	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	527007	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	434117	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	429978	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	2492	1.09	ng/uL	0.00
5) Phenol-d5	6.83	99	67614	7.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	37795	7.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	55814	7.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	45862	6.11	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	26438	7.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	18937	4.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	58793	7.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	68722	8.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	185552	8.60	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	194262	7.49	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	16632	4.55	ng/ul	0.00
57) Fluorene-d10	15.31	176	130822	7.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	447	0.13	ng/ul	0.00
70) Anthracene-d10	17.16	188	185400	7.49	ng/ul	0.00
78) Pyrene-d10	19.46	212	162201	8.18	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	127640	5.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.77	163	70945	3.23	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072015\
Data File : BM001994.D
Acq On : 21 Jul 2015 03:30
Operator : TP/UM
Sample : G3000-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C02B9

Quant Time: Jul 21 04:05:54 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 21 01:37:44 2015
Response via : Initial Calibration

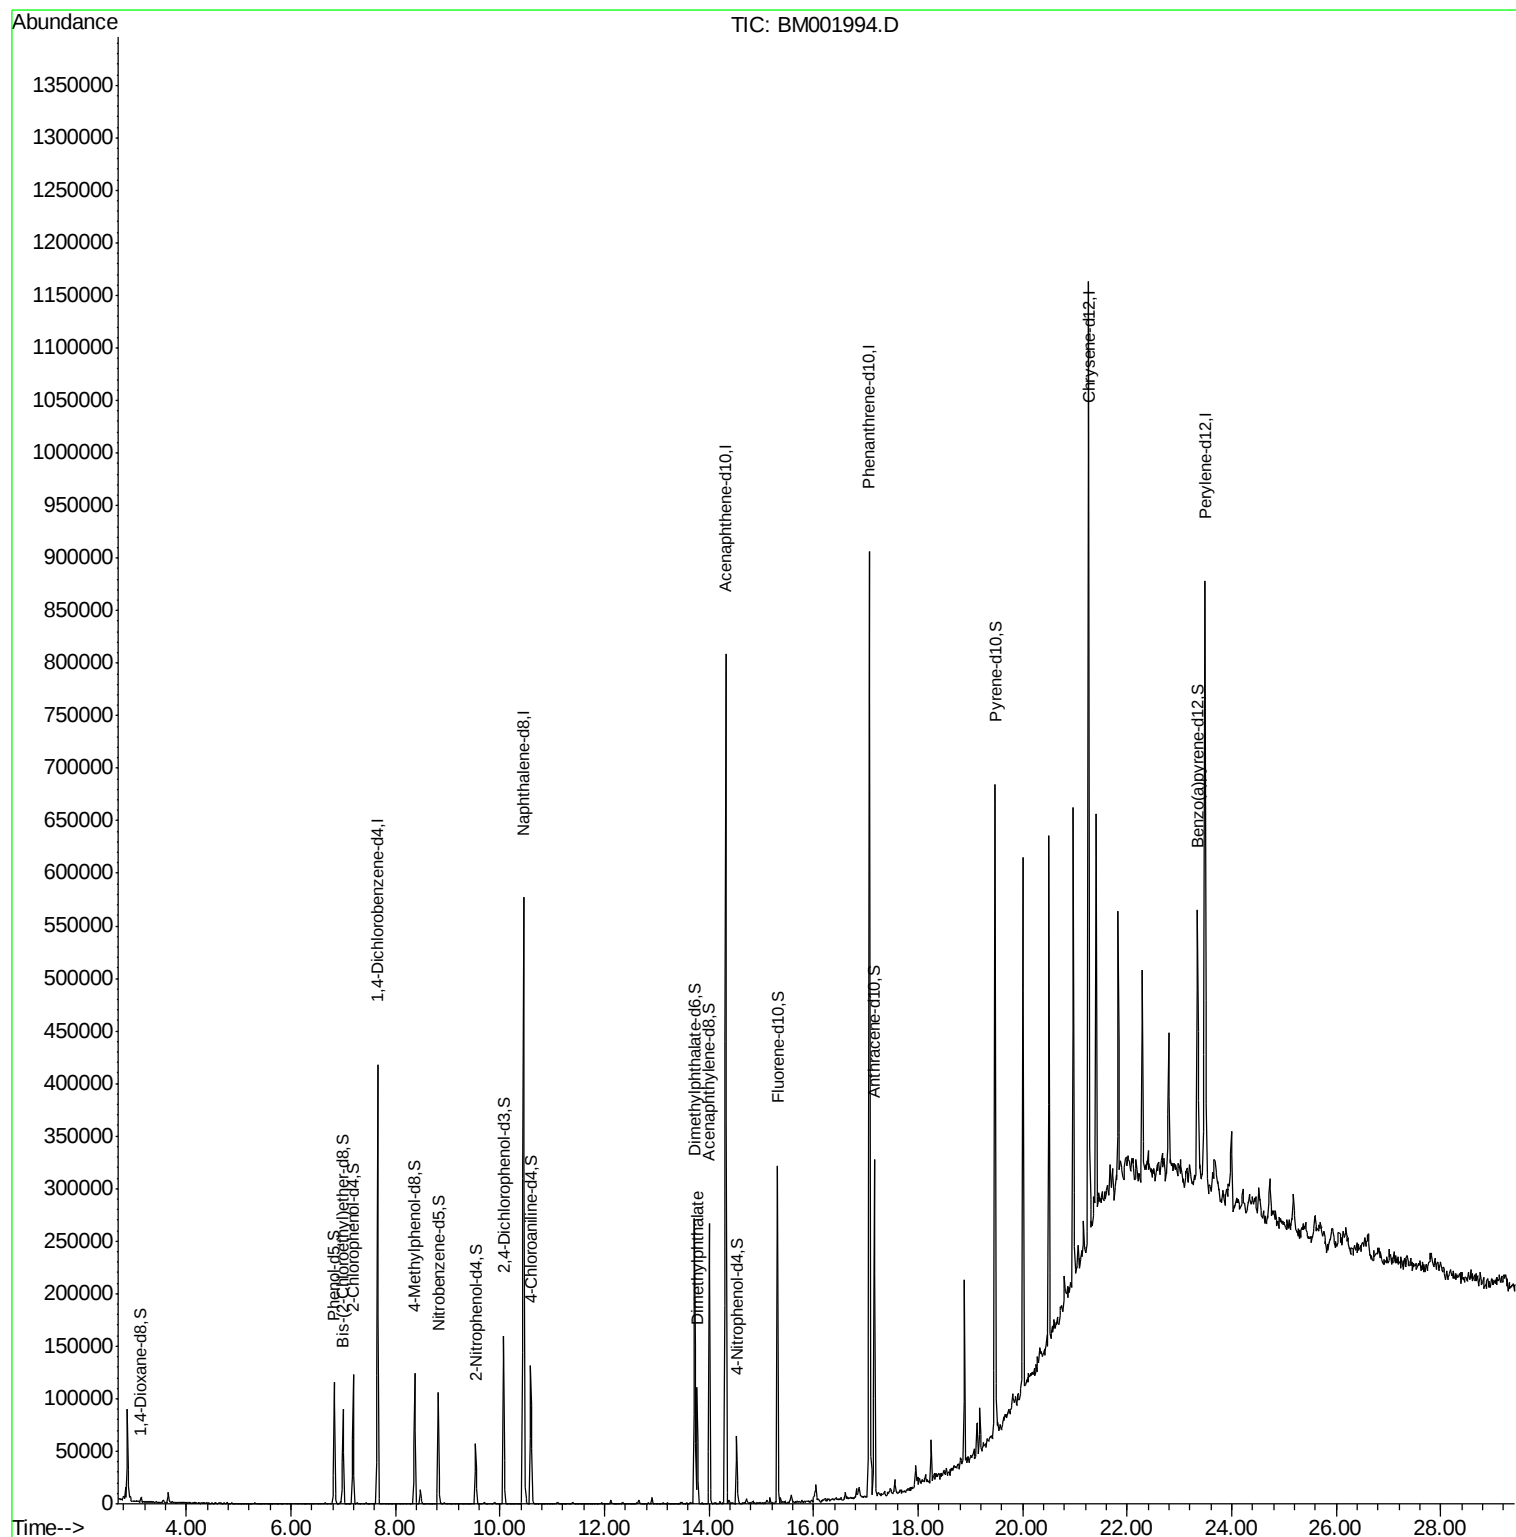

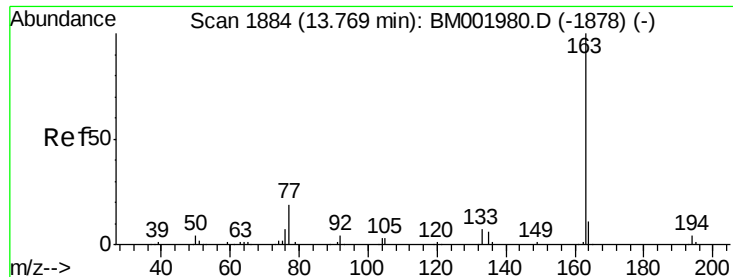

#44

Dimethylphthalate

Concen: 3.23 ng/ul

RT: 13.77 min Scan# 1884

Delta R.T. -0.00 min

Lab File: BM001994.D


Acq: 21 Jul 2015 03:30

Instrument :

BNA_M

ClientSampleId :

C02B9

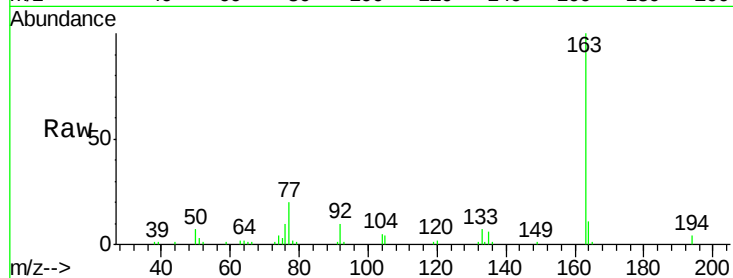


Tgt Ion:163 Resp: 70945

Ion Ratio Lower Upper

163 100

194 4.4 3.3 4.9

164 11.0 7.6 11.4

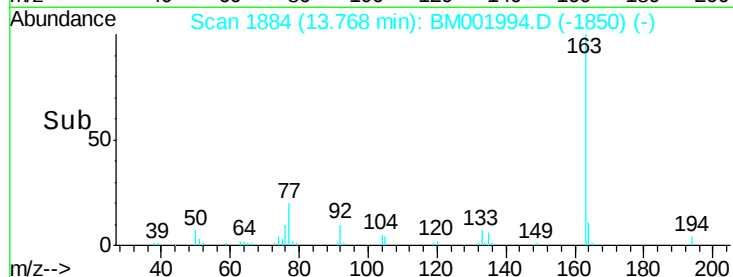

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

