

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072015\
 Data File : BM001969.D
 Acq On : 20 Jul 2015 12:00
 Operator : TP/UM
 Sample : PB84576BL
 Misc : SBLK76
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.787	12	17	21	rBV4	4671	7726	0.40%	0.040%
2	2.869	28	31	38	rVB	24813	34287	1.75%	0.176%
3	3.134	72	76	82	rVB	15470	18161	0.93%	0.093%
4	3.681	165	169	174	rVB3	4533	6091	0.31%	0.031%
5	6.822	697	703	712	rVB	287795	439344	22.48%	2.256%
6	6.992	725	732	742	rVB	225730	346658	17.74%	1.780%
7	7.181	758	764	773	rVB	288803	462378	23.66%	2.374%
8	7.651	838	844	852	rBV	307296	468115	23.96%	2.404%
9	8.357	958	964	972	rBV	392367	586774	30.03%	3.013%
10	8.816	1034	1042	1049	rVB	278664	448501	22.95%	2.303%
11	9.533	1157	1164	1172	rVB	236512	384958	19.70%	1.977%
12	10.063	1246	1254	1265	rBB	381005	624982	31.98%	3.209%
13	10.439	1310	1318	1326	rBB	415723	700732	35.86%	3.598%
14	10.580	1336	1342	1350	rBV	374640	626445	32.06%	3.217%
15	13.721	1870	1876	1882	rBV	766575	1015316	51.96%	5.214%
16	14.004	1917	1924	1930	rBV	793577	1180084	60.39%	6.060%
17	14.310	1970	1976	1983	rVB2	688302	1031780	52.80%	5.299%
18	14.515	2005	2011	2023	rBV	297715	420948	21.54%	2.162%
19	15.304	2139	2145	2152	rVB	1061168	1500593	76.80%	7.706%
20	15.433	2161	2167	2173	rBV	244683	333418	17.06%	1.712%
21	15.545	2181	2186	2192	rVB2	3820	4440	0.23%	0.023%
22	16.839	2401	2406	2411	rVB2	2252	3159	0.16%	0.016%
23	17.056	2437	2443	2449	rBV	904598	1245257	63.73%	6.395%
24	17.156	2454	2460	2469	rBV	1249252	1718068	87.93%	8.823%
25	18.021	2604	2607	2613	rVB3	1293	2355	0.12%	0.012%
26	19.350	2827	2833	2839	rBV	8369	11213	0.57%	0.058%
27	19.462	2846	2852	2861	rBV	1484059	1953989	100.00%	10.034%
28	20.039	2945	2950	2953	rBV4	2030	3440	0.18%	0.018%
29	20.933	3098	3102	3103	rBV2	2530	3159	0.16%	0.016%
30	21.056	3119	3123	3131	rBV2	10266	13551	0.69%	0.070%
31	21.180	3142	3144	3147	rVB4	2141	2126	0.11%	0.011%
32	21.262	3153	3158	3164	rBV	1041704	1293848	66.22%	6.644%
33	23.350	3505	3513	3522	rBV2	836866	1513614	77.46%	7.773%
34	23.491	3529	3537	3552	rVB2	569713	1067458	54.63%	5.482%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072015\
Data File : BM001969.D
Acq On : 20 Jul 2015 12:00
Operator : TP/UM
Sample : PB84576BL
Misc : SBLK76
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK76

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Title : SVOA CALIBRATION


Sum of corrected areas: 19472968

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072015\
Data File : BM001969.D
Acq On : 20 Jul 2015 12:00
Operator : TP/UM
Sample : PB84576BL
Misc : SBLK76
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK76

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

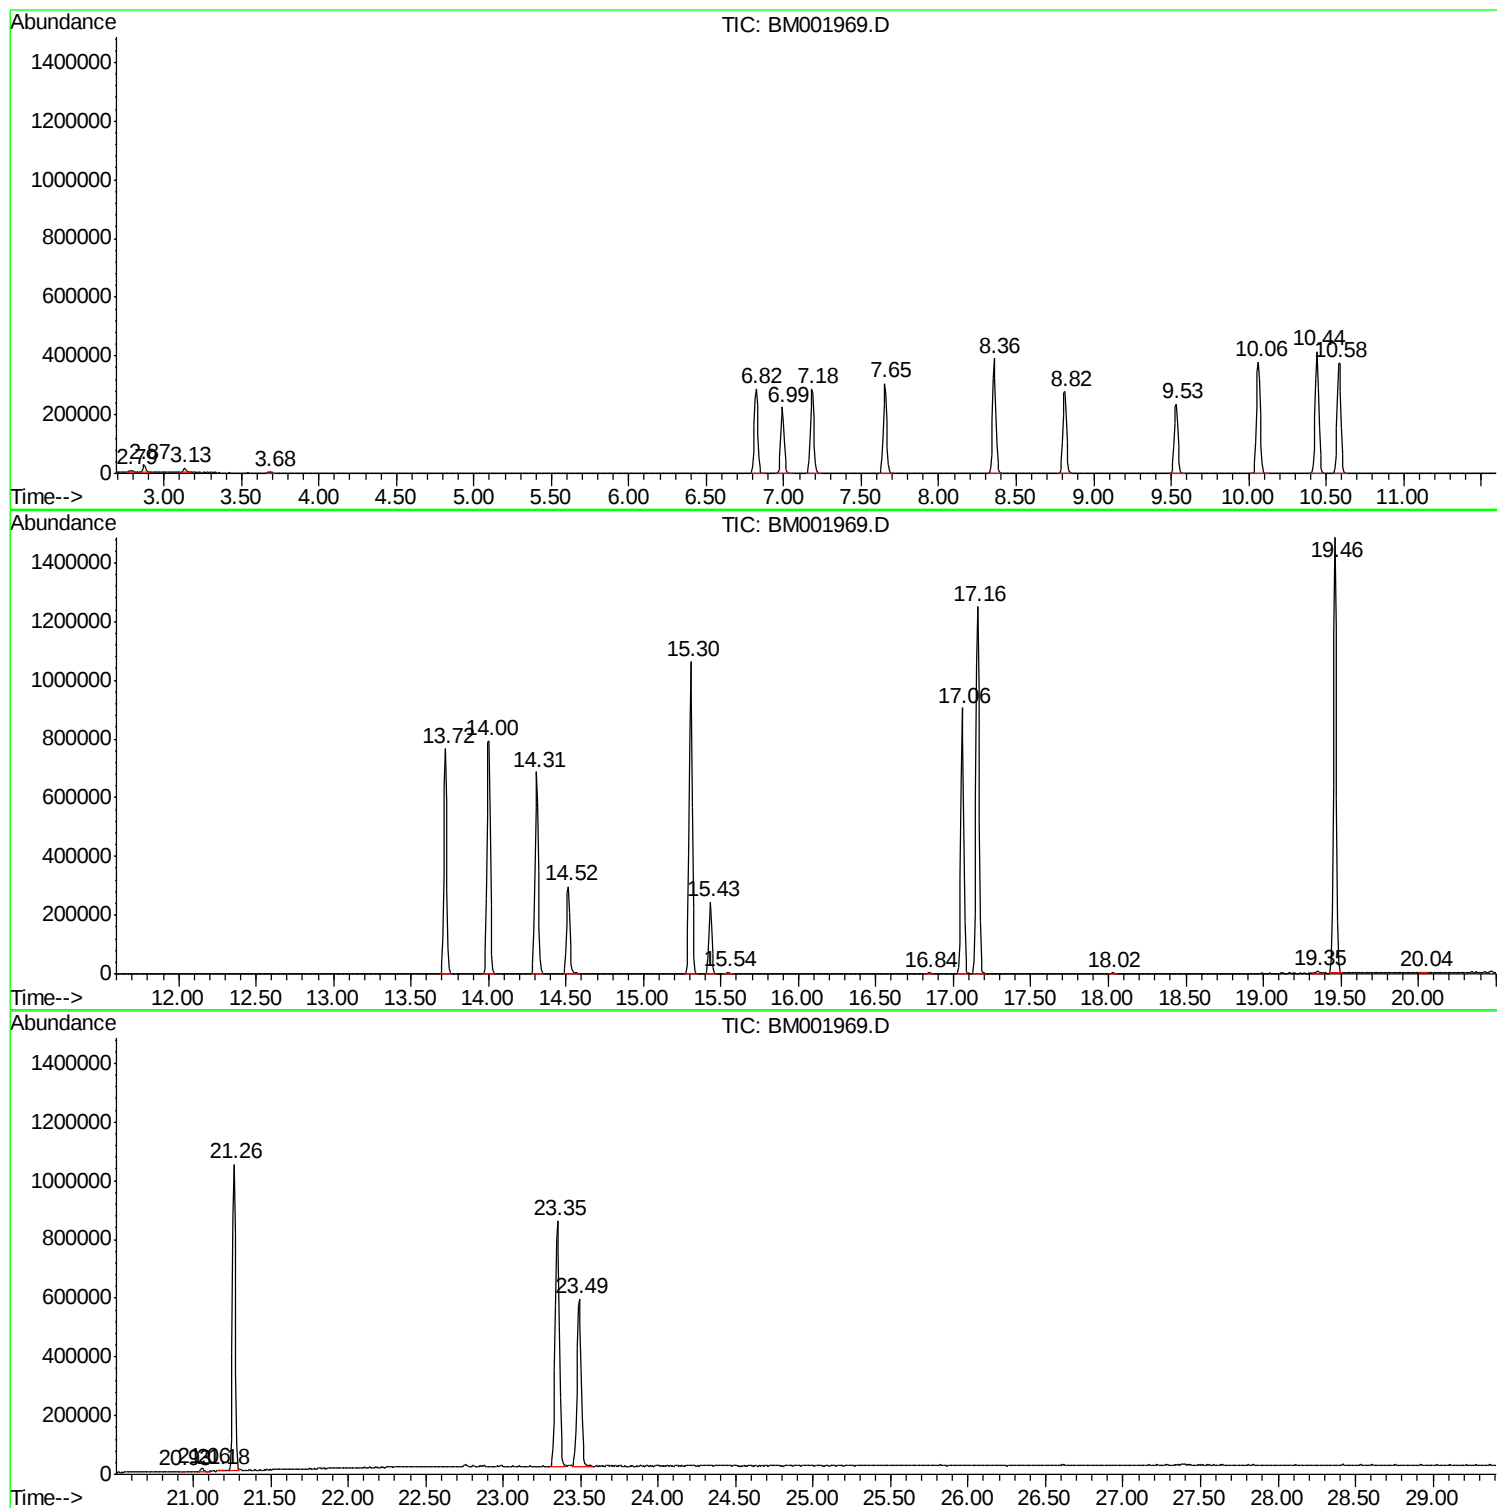

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072015\
Data File : BM001969.D
Acq On : 20 Jul 2015 12:00
Operator : TP/UM
Sample : PB84576BL
Misc : SBLK76
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK76

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072015\
Data File : BM001969.D
Acq On : 20 Jul 2015 12:00
Operator : TP/UM
Sample : PB84576BL
Misc : SBLK76
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK76

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc