

Data Path : Z:\HPCHEM1\BNA_M\Data\BM072015\
 Data File : BM001971.D
 Acq On : 20 Jul 2015 13:14
 Operator : TP/UM
 Sample : PB84556BL
 Misc : SBLK94
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK94

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.869	27	31	40	rVB	22698	31181	1.70%	0.172%
2	3.134	72	76	82	rVB2	12333	17344	0.94%	0.096%
3	3.681	166	169	176	rBV	4100	5312	0.29%	0.029%
4	6.822	696	703	710	rBV	256537	397134	21.59%	2.189%
5	6.993	726	732	739	rBV	204416	309480	16.82%	1.706%
6	7.181	758	764	773	rVB	269667	413782	22.49%	2.280%
7	7.651	837	844	851	rBB	272092	418075	22.73%	2.304%
8	8.357	957	964	972	rBV	345186	535907	29.13%	2.953%
9	8.810	1035	1041	1050	rVB	249462	409429	22.26%	2.256%
10	9.528	1157	1163	1172	rBB	212962	357306	19.42%	1.969%
11	10.063	1246	1254	1263	rBV	357264	581600	31.62%	3.205%
12	10.439	1311	1318	1329	rBB	389666	641576	34.88%	3.536%
13	10.581	1336	1342	1353	rBB	358860	588916	32.01%	3.246%
14	13.722	1870	1876	1882	rBV	714714	928419	50.47%	5.117%
15	13.998	1916	1923	1930	rBV	763952	1106423	60.15%	6.098%
16	14.310	1969	1976	1984	rVB2	648676	959894	52.18%	5.290%
17	14.516	2005	2011	2026	rVB	273839	398305	21.65%	2.195%
18	15.304	2139	2145	2152	rVB	992985	1411147	76.71%	7.777%
19	15.433	2161	2167	2176	rVB	227232	314957	17.12%	1.736%
20	15.539	2182	2185	2188	rBV	3091	3634	0.20%	0.020%
21	16.845	2403	2407	2411	rVB	1936	2805	0.15%	0.015%
22	17.057	2437	2443	2449	rBV2	836163	1167539	63.47%	6.434%
23	17.157	2453	2460	2469	rBV	1132174	1603771	87.18%	8.838%
24	19.351	2828	2833	2836	rBV	6504	9143	0.50%	0.050%
25	19.462	2845	2852	2863	rBV	1381196	1839510	100.00%	10.138%
26	20.380	3005	3008	3011	rBV2	1157	1880	0.10%	0.010%
27	21.056	3119	3123	3126	rBV2	8829	11113	0.60%	0.061%
28	21.262	3152	3158	3163	rBV	998049	1240650	67.44%	6.837%
29	22.756	3408	3412	3416	rVB4	6795	9832	0.53%	0.054%
30	23.344	3505	3512	3523	rVB2	782819	1428919	77.68%	7.875%
31	23.492	3529	3537	3546	rVB	531206	1000495	54.39%	5.514%


Sum of corrected areas: 18145478

Data Path : Z:\HPCHEM1\BNA_M\Data\BM072015\
Data File : BM001971.D
Acq On : 20 Jul 2015 13:14
Operator : TP/UM
Sample : PB84556BL
Misc : SBLK94
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK94

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

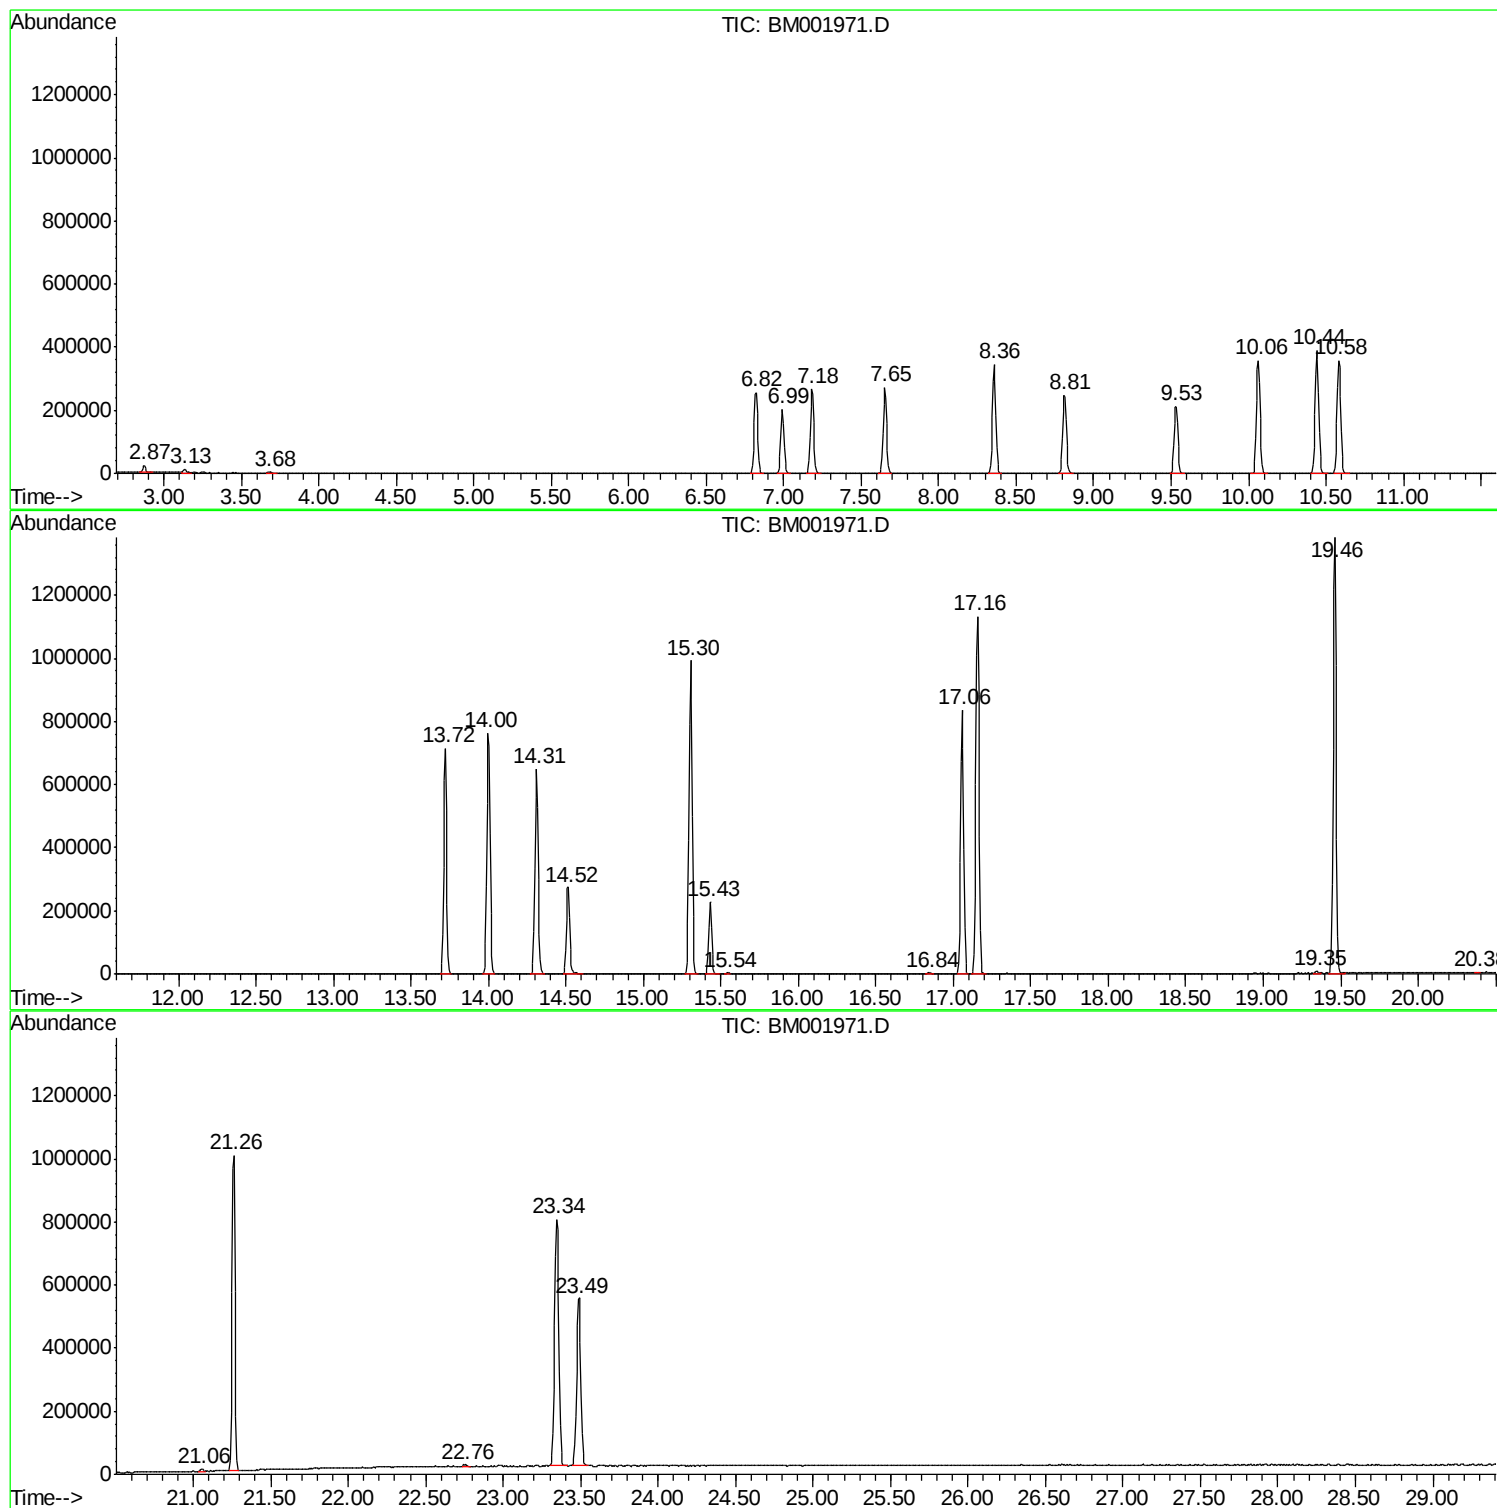

Data Path : Z:\HPCHEM1\BNA_M\Data\BM072015\
Data File : BM001971.D
Acq On : 20 Jul 2015 13:14
Operator : TP/UM
Sample : PB84556BL
Misc : SBLK94
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK94

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM072015\
Data File : BM001971.D
Acq On : 20 Jul 2015 13:14
Operator : TP/UM
Sample : PB84556BL
Misc : SBLK94
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK94

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc