


Data Path : Z:\HPCHEM1\BNA_M\Data\BM072015\
Data File : BM001967.D
Acq On : 20 Jul 2015 10:10
Operator : TP/UM
Sample : DFTPP77
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP77

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\Methods\SOM02.2-EPA-BM042815.M
Title : SVOA CALIBRATION
Last Update : Tue Apr 28 06:36:34 2015

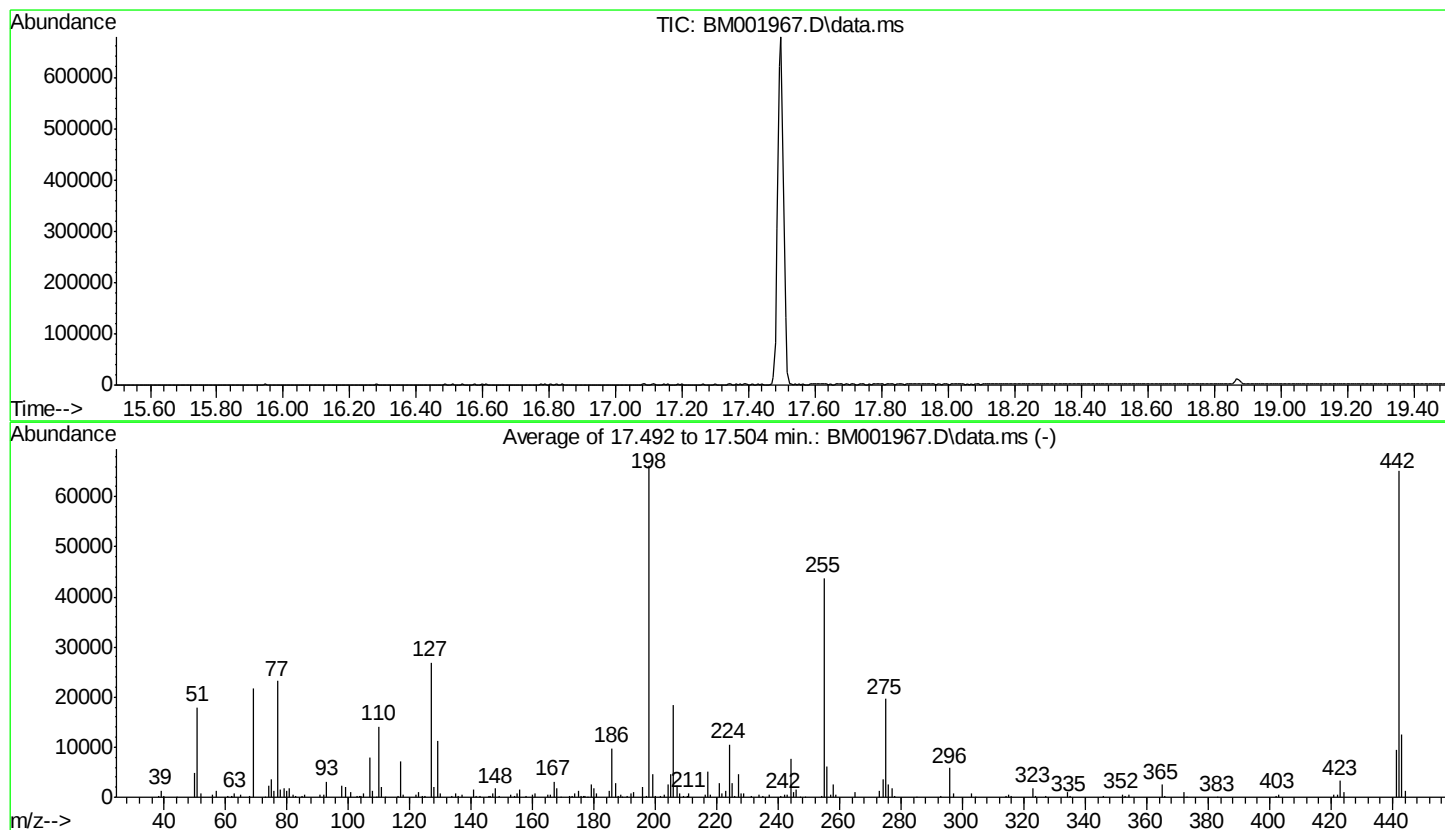

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	17949	PASS
68	69	0.00	2	1.5	334	PASS
69	198	0.00	100	33.0	21828	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.7	26960	PASS
197	198	0.00	2	0.6	372	PASS
198	198	100	100	100.0	66210	PASS
199	198	5	9	6.8	4488	PASS
275	198	10	60	29.6	19622	PASS
365	198	1	100	3.8	2546	PASS
441	443	0.01	100	75.4	9488	PASS
442	198	50	100	98.6	65304	PASS
443	442	15	24	19.3	12583	PASS

m/z	Abundance
38.10	436.0
39.00	1812.0
40.00	428.0
44.00	803.0
50.10	6108.0
51.00	22912.0
52.00	949.0
55.90	902.0
57.00	1722.0
61.00	476.0
61.90	441.0
63.00	966.0
65.00	491.0
68.00	472.0
69.00	27656.0
72.90	365.0
74.00	2965.0
75.00	4382.0
76.00	1520.0
77.00	28496.0
78.00	1976.0
79.00	2445.0
80.00	1562.0
81.00	2144.0
82.00	775.0
83.00	400.0
84.90	434.0
86.00	555.0
91.00	625.0
91.90	666.0
93.00	3870.0
98.00	2853.0
99.00	2629.0
100.90	1277.0
102.90	455.0
103.80	847.0
105.00	728.0
107.00	9960.0
108.00	1498.0
110.00	17448.0
111.00	2560.0
116.00	590.0
117.00	8854.0
118.00	489.0
121.90	681.0
123.00	1007.0
124.00	483.0
124.90	523.0
127.00	32592.0
128.00	2305.0
129.00	13167.0
130.00	1032.0
133.90	338.0
135.00	1010.0
136.00	480.0
136.90	683.0
141.00	1696.0
141.80	557.0
145.90	417.0
146.90	1025.0
148.00	1970.0
149.00	384.0
152.90	592.0
153.90	435.0
155.00	949.0
156.00	1686.0
157.90	425.0
160.00	686.0
161.00	860.0
165.00	699.0
165.90	578.0
167.00	3484.0
168.00	1967.0
169.00	372.0
172.00	385.0
173.90	804.0
174.90	1383.0
175.90	397.0
176.80	524.0
179.00	3024.0
180.00	1898.0
181.00	700.0
185.00	1371.0
186.00	11034.0
187.00	3268.0
188.00	375.0
188.90	853.0
190.90	420.0
192.00	884.0
193.00	1049.0
196.00	2187.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77

197.00	490.0
197.90	72392.0
198.90	5534.0
199.90	482.0
201.60	305.0
203.00	525.0
204.00	2792.0
205.00	5120.0
206.00	20264.0
207.10	3007.0
208.00	861.0
208.90	370.0
211.00	901.0
216.00	356.0
217.00	5518.0
218.00	489.0
221.00	3386.0
221.90	719.0
223.00	1332.0
224.00	11342.0
225.00	2880.0
225.90	327.0
227.00	5339.0
228.00	685.0
229.00	879.0
231.00	560.0
234.00	332.0
235.00	403.0
236.90	629.0
242.00	583.0
242.90	638.0
244.00	8156.0
245.10	1321.0
246.00	1777.0
246.90	394.0
248.90	328.0
254.10	351.0
255.00	45584.0
256.00	6421.0
257.00	540.0
257.90	2715.0
259.00	487.0
265.00	1144.0
273.00	1444.0
274.00	3756.0
275.00	20152.0
276.00	2804.0
277.00	1844.0
278.00	332.0
293.00	431.0
296.00	5996.0
297.00	774.0
303.00	658.0
315.00	493.0
316.10	411.0
323.00	1690.0
323.90	307.0
326.90	345.0
334.00	1039.0
345.90	327.0
352.10	512.0
353.10	309.0
354.00	513.0
364.90	2357.0
366.00	319.0
372.00	809.0
402.90	529.0
420.90	337.0
421.90	422.0
423.00	2954.0
424.00	936.0
441.10	8072.0
442.10	55120.0
443.10	10869.0
444.10	1080.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77

m/z	Abundance
39.10	1657.0
44.00	722.0
50.00	5471.0
51.00	20472.0
52.00	1030.0
55.90	650.0
57.00	1378.0
61.00	393.0
62.10	317.0
63.00	1107.0
65.00	649.0
67.90	531.0
69.00	25408.0
74.00	2775.0
75.00	4074.0
76.00	1396.0
77.00	26448.0
78.00	1857.0
79.00	2218.0
80.00	1708.0
81.00	2202.0
82.00	570.0
83.00	467.0
85.00	503.0
86.00	766.0
91.00	553.0
91.90	602.0
93.00	3685.0
98.00	3052.0
99.00	2232.0
101.00	1048.0
102.90	440.0
104.00	705.0
105.00	887.0
107.00	9272.0
108.00	1422.0
109.10	328.0
110.00	16039.0
111.00	2384.0
111.90	301.0
116.10	544.0
117.00	8376.0
118.00	719.0
121.90	749.0
123.00	1174.0
124.10	377.0
124.90	439.0
127.00	31736.0
128.10	2552.0
129.00	13686.0
129.90	1007.0
133.90	508.0
135.00	943.0
136.00	336.0
136.90	568.0
140.90	2013.0
141.90	516.0
143.00	464.0
146.10	444.0
147.00	875.0
148.00	2032.0
149.00	470.0
152.90	591.0
154.00	557.0
155.00	973.0
156.00	1671.0
160.00	460.0
161.10	697.0
165.00	611.0
166.00	608.0
167.00	3655.0
168.00	2333.0
172.00	427.0
172.90	440.0
173.90	818.0
175.00	1682.0
175.90	490.0
177.00	633.0
178.00	388.0
179.00	2796.0
180.00	2256.0
181.00	871.0
185.10	1477.0
186.00	11892.0
187.00	3213.0
188.00	402.0
188.80	650.0
190.80	353.0
192.00	952.0
193.00	1074.0
195.90	2404.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77

197.10	627.0
198.00	80088.0
199.00	5304.0
200.00	410.0
201.40	548.0
202.90	597.0
204.00	3123.0
205.00	5750.0
206.00	21200.0
207.00	3333.0
208.00	1154.0
209.00	361.0
210.20	443.0
210.90	958.0
216.00	533.0
217.00	6104.0
217.90	809.0
221.00	2808.0
221.90	632.0
222.90	1541.0
224.00	12322.0
225.00	3652.0
225.90	452.0
227.00	5483.0
228.00	946.0
228.90	1067.0
231.10	439.0
233.90	470.0
235.00	394.0
236.90	433.0
241.00	489.0
242.00	916.0
243.00	753.0
244.00	9512.0
245.00	1336.0
246.00	1834.0
254.10	460.0
255.00	52808.0
256.00	7576.0
257.00	816.0
258.00	3386.0
258.90	481.0
265.00	1490.0
273.00	1285.0
274.00	4236.0
275.00	23544.0
276.00	3231.0
276.90	2100.0
277.80	432.0
285.00	369.0
293.00	461.0
296.00	6541.0
297.00	887.0
303.00	823.0
304.00	313.0
314.00	471.0
314.90	528.0
315.90	459.0
323.00	2314.0
326.90	391.0
334.00	1095.0
334.90	413.0
345.90	515.0
351.90	682.0
352.90	461.0
354.00	633.0
365.00	2915.0
365.90	429.0
372.00	1271.0
372.90	321.0
383.00	316.0
402.00	370.0
403.00	660.0
421.00	453.0
422.00	532.0
423.00	3945.0
424.00	1148.0
441.10	11408.0
442.10	78680.0
443.10	14993.0
444.00	1335.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77

m/z	Abundance
39.10	676.0
39.90	326.0
44.00	792.0
50.00	2726.0
51.10	10465.0
52.00	599.0
56.00	313.0
57.00	871.0
63.10	509.0
65.00	313.0
69.00	12420.0
74.00	1259.0
75.00	2278.0
76.10	727.0
77.10	14531.0
78.00	923.0
79.00	1024.0
79.90	936.0
81.00	1131.0
85.90	448.0
90.90	398.0
93.00	1733.0
98.00	1364.0
99.00	1103.0
101.00	623.0
104.00	364.0
105.00	487.0
107.00	4849.0
107.90	697.0
110.00	8785.0
111.00	1383.0
117.00	4099.0
121.90	336.0
123.00	591.0
127.00	16552.0
128.00	1402.0
129.00	6999.0
129.90	506.0
134.90	562.0
136.00	349.0
137.00	368.0
141.00	1206.0
146.90	627.0
148.00	1212.0
154.90	550.0
156.00	893.0
159.90	370.0
160.90	454.0
167.00	2217.0
168.00	1225.0
173.80	481.0
175.10	696.0
176.90	435.0
179.00	1828.0
180.00	1242.0
181.00	556.0
185.00	827.0
186.00	6620.0
187.00	1955.0
189.10	399.0
192.00	686.0
192.90	731.0
195.90	1396.0
197.90	46152.0
198.90	2628.0
202.90	304.0
203.90	1910.0
205.00	2935.0
206.00	13757.0
207.00	1992.0
207.90	592.0
211.10	478.0
216.10	302.0
216.90	3696.0
217.90	424.0
221.00	2463.0
221.70	666.0
222.90	801.0
224.00	8127.0
225.00	2145.0
227.00	3173.0
228.00	416.0
228.90	669.0
233.90	403.0
237.00	314.0
241.90	379.0
243.10	379.0
244.00	5629.0
245.00	646.0
246.00	1086.0
255.00	33048.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77

256.00	4644.0
256.90	487.0
258.10	1917.0
258.90	329.0
265.10	714.0
273.00	994.0
274.00	2403.0
275.00	15170.0
276.00	1976.0
277.00	1265.0
296.00	4755.0
296.90	772.0
303.10	472.0
314.90	524.0
323.00	1475.0
324.00	311.0
334.00	1049.0
352.00	524.0
354.00	396.0
365.00	2367.0
365.90	370.0
372.00	849.0
401.90	360.0
403.00	506.0
421.00	431.0
422.10	577.0
423.00	2795.0
424.00	841.0
441.10	8986.0
442.10	62112.0
443.10	11889.0
444.10	1068.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77

m/z	Abundance
44.00	728.0
207.00	438.0

Instrument :
BNA_M
ClientSampleId :
DFTPP77