
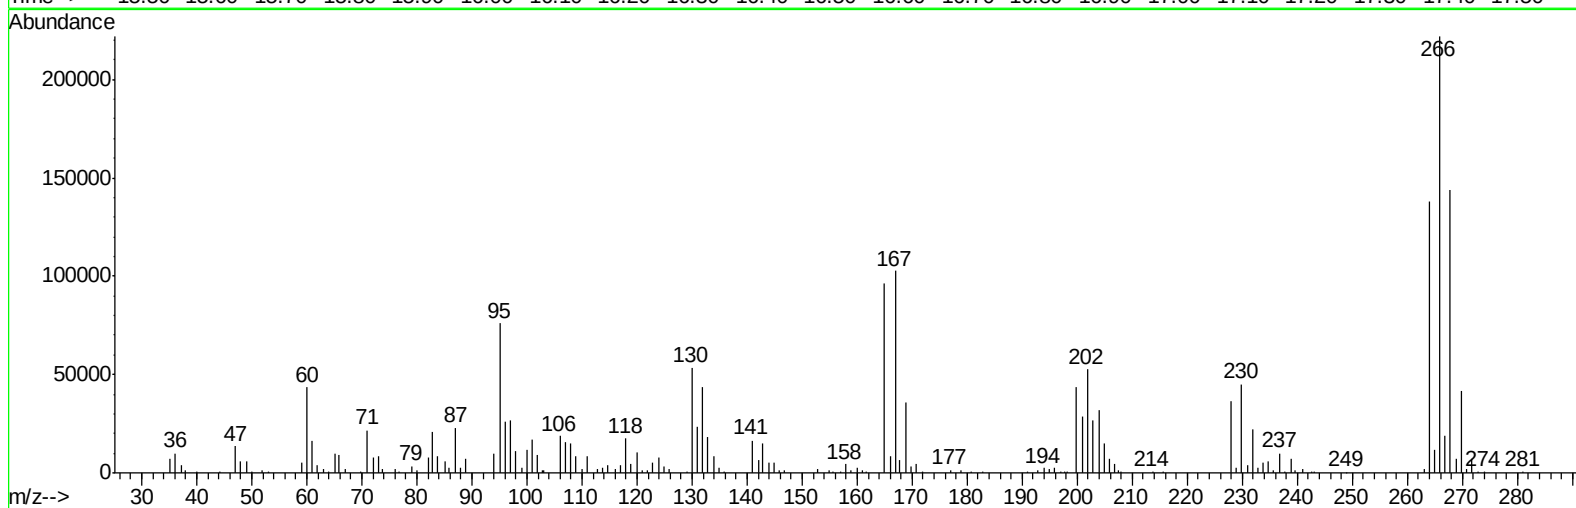


Data File : BM010905.D
Acq On : 20 Jul 2017 12:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 06:09:09 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

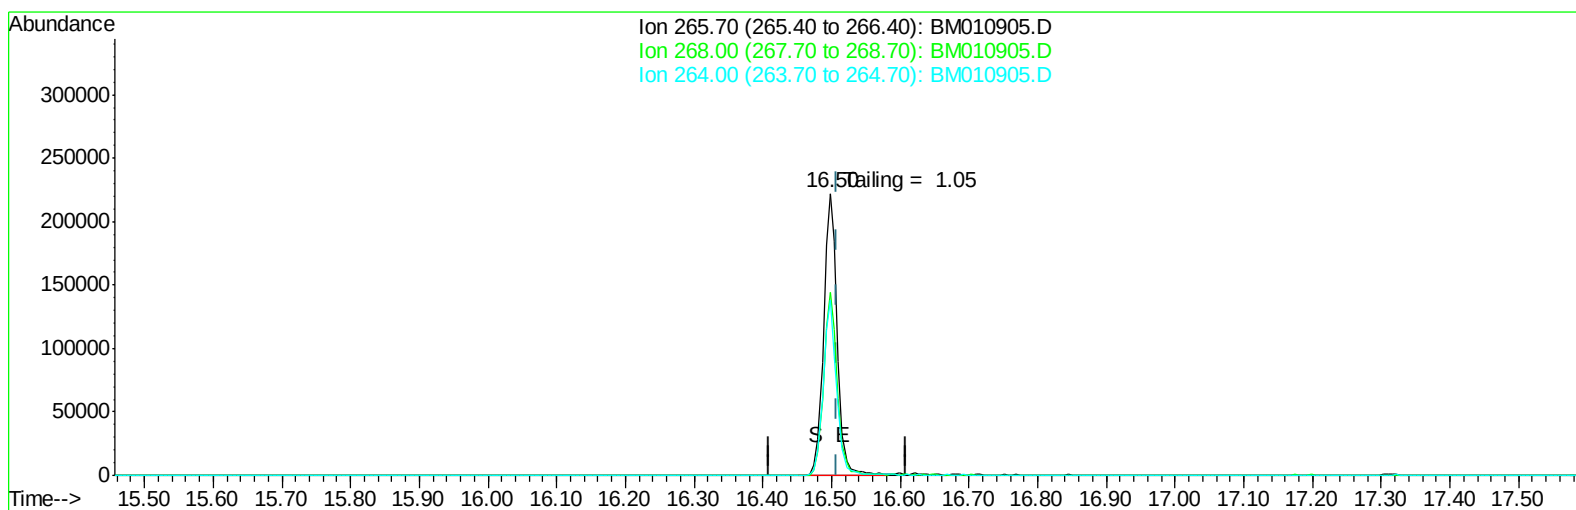

TIC: BM010905.D

(69) Pentachlorophenol (C)

16.498min (-0.011) 0.00ng

response 308318

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.85
264.00	61.20	62.28
0.00	0.00	0.00