
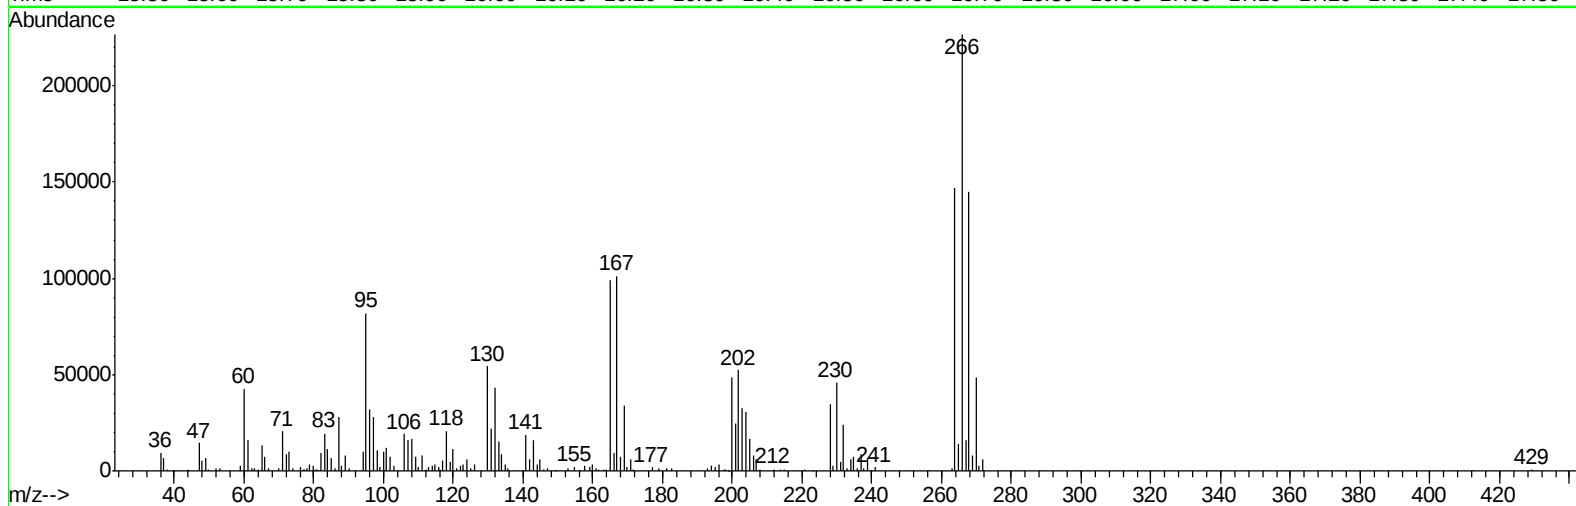


Data File : BM010924.D
Acq On : 21 Jul 2017 00:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 06:10:48 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

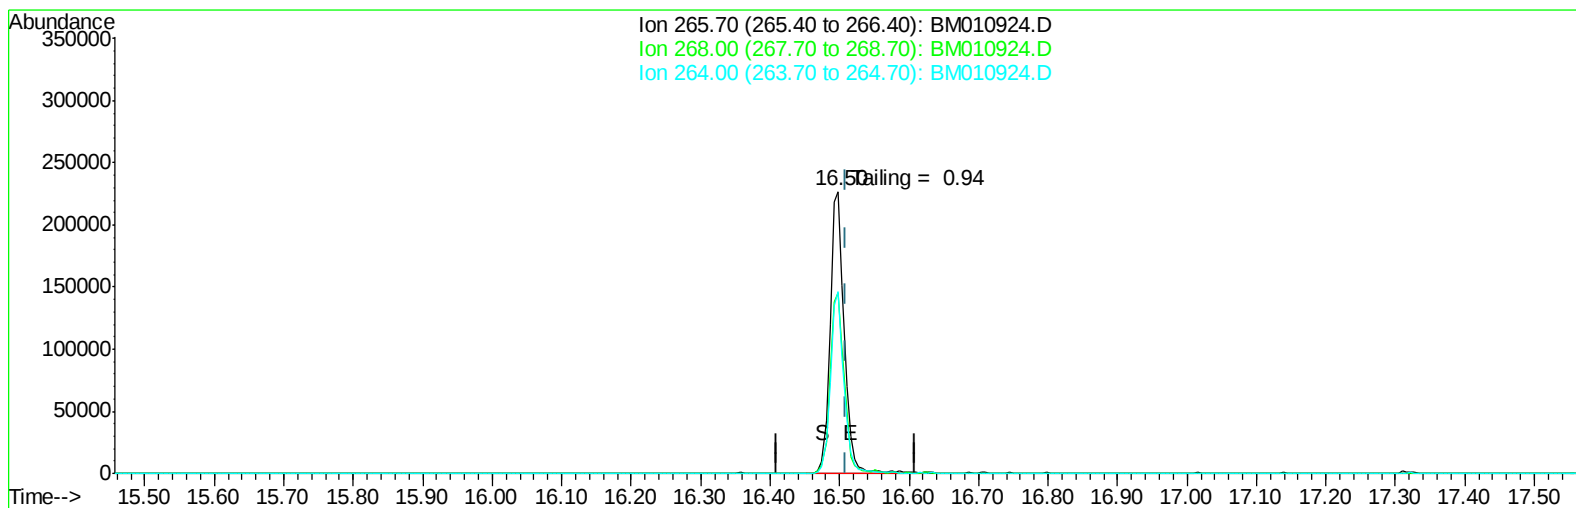

TIC: BM010924.D

(69) Pentachlorophenol (C)

16.498min (-0.011) 0.00ng

response 316804

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.95
264.00	61.20	64.71
0.00	0.00	0.00