
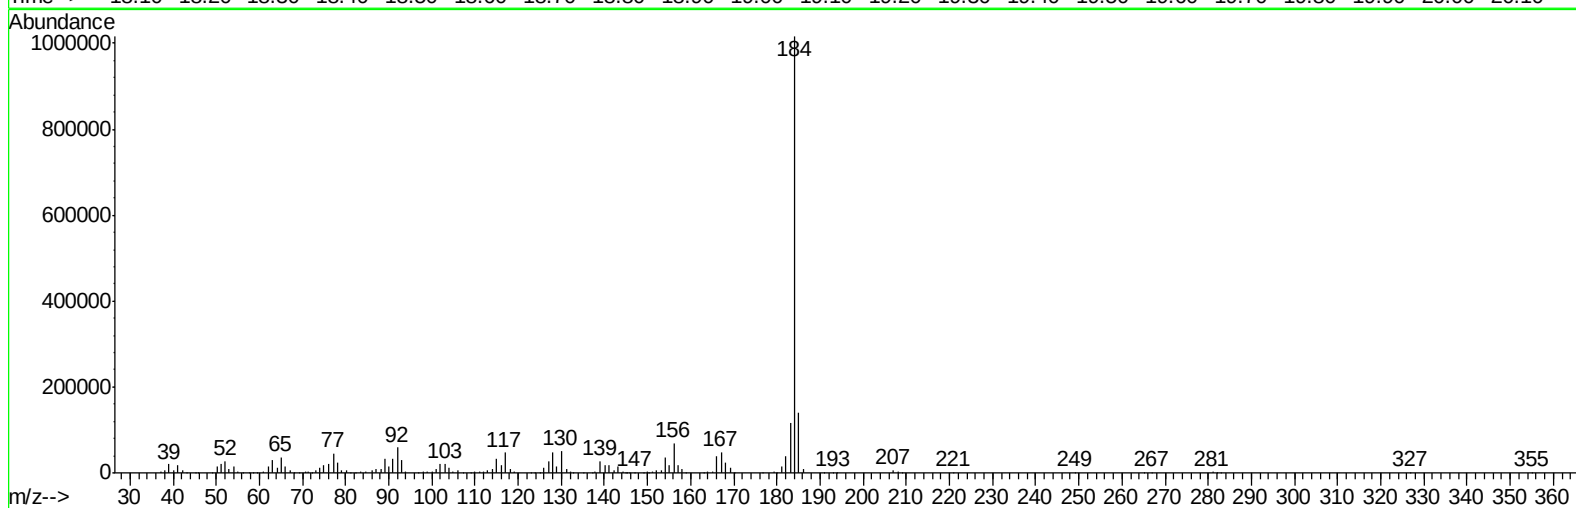


Data File : BM010924.D
Acq On : 21 Jul 2017 00:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 06:10:48 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

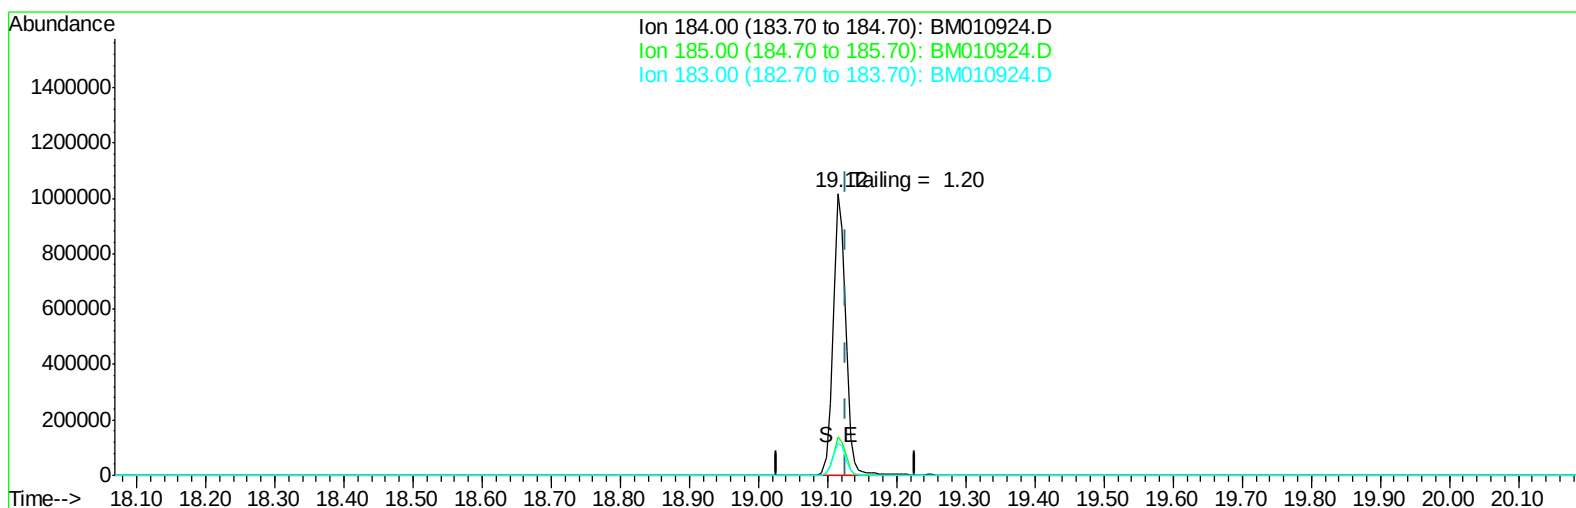

TIC: BM010924.D

(76) Benzidine

19.115min (-0.011) 42579.49ng

response 1270471

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.71
183.00	11.10	11.37
0.00	0.00	0.00