


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.43 min Scan# 773
Delta R.T. -0.02 min
Lab File: BM010933.D
Acq: 21 Jul 2017 08:59

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:152 Resp: 201075
Ion Ratio Lower Upper
152 100
150 161.4 119.5 179.3
115 72.1 43.0 64.4#

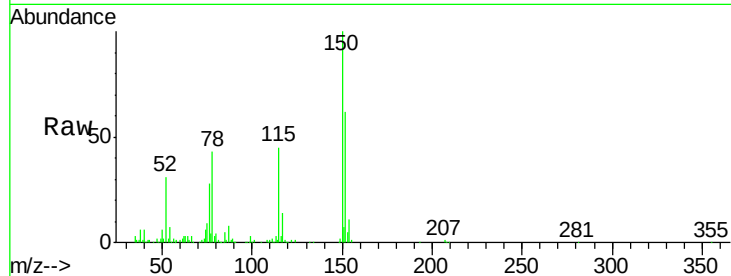


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

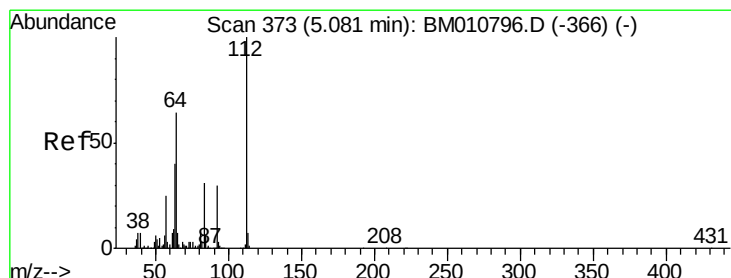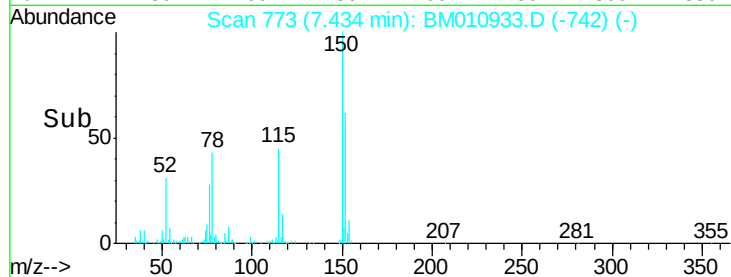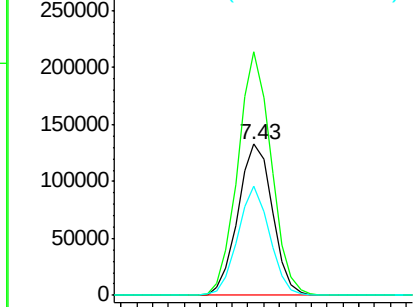

#5

2-Fluorophenol
Concen: 139.538 ng
RT: 5.08 min Scan# 372
Delta R.T. -0.00 min
Lab File: BM010933.D
Acq: 21 Jul 2017 08:59

Tgt Ion:112 Resp: 1693799
Ion Ratio Lower Upper
112 100
64 64.8 38.6 57.8#
63 42.8 19.3 28.9#

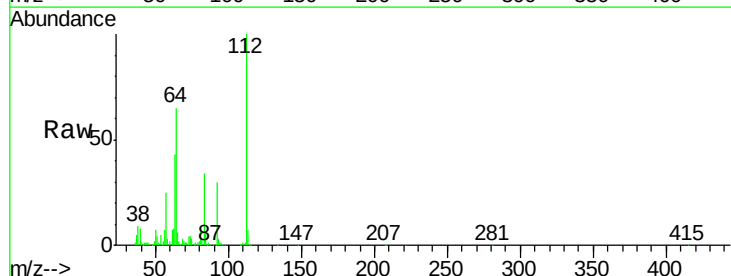

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

