





#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.19 min Scan# 1242
Delta R.T. -0.02 min
Lab File: BM010933.D
Acq: 21 Jul 2017 08:59

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:	136	Resp:	765268
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.7	13.1
54	9.1	4.6	6.8#
68	6.2	3.7	5.5#

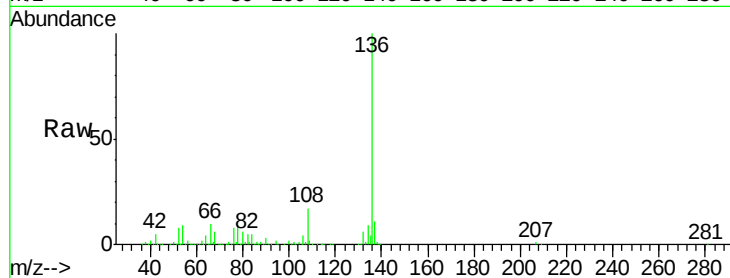


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

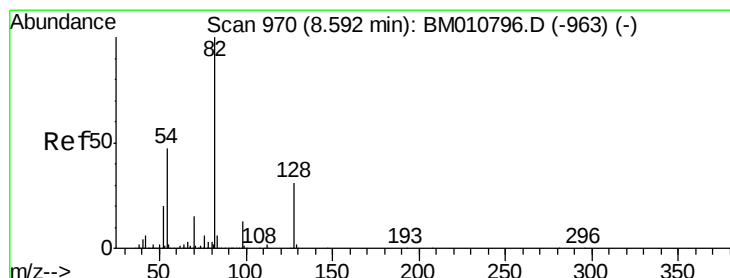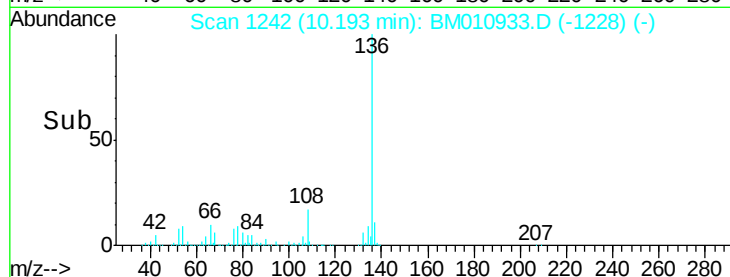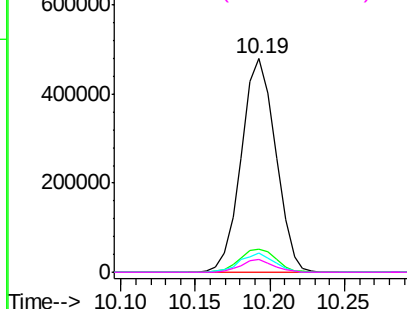

#23
Nitrobenzene-d5
Concen: 103.174 ng
RT: 8.58 min Scan# 968
Delta R.T. -0.01 min
Lab File: BM010933.D
Acq: 21 Jul 2017 08:59

Tgt Ion:	82	Resp:	2054131
Ion	Ratio	Lower	Upper
82	100		
128	28.1	32.8	49.2#
54	48.4	40.6	60.8

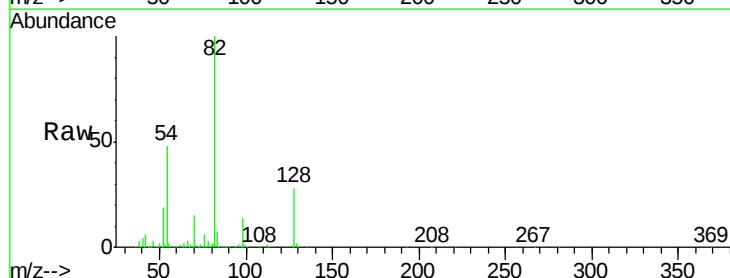

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

