
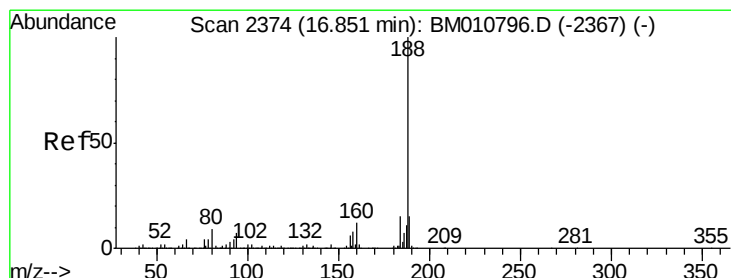
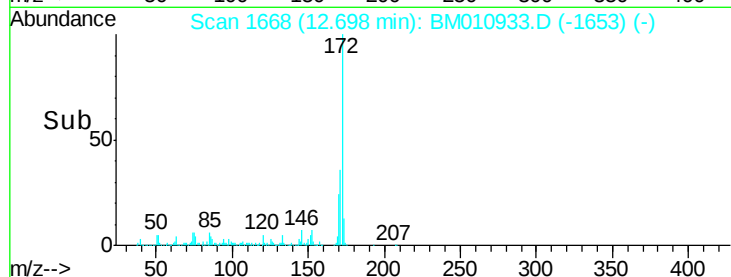
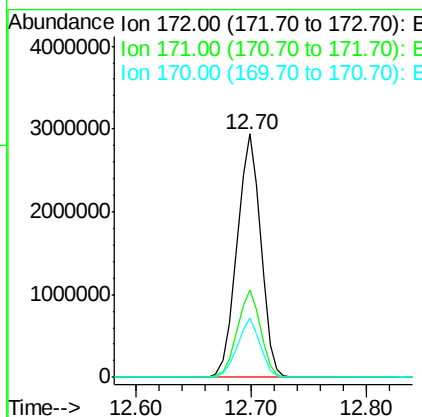


#44
 2-Fluorobiphenyl
 Concen: 102.026 ng
 RT: 12.70 min Scan# 1668
 Delta R.T. -0.01 min
 Lab File: BM010933.D
 Acq: 21 Jul 2017 08:59

Instrument :
 BNA_M
 ClientSampleId :

Tgt Ion:172 Resp: 4171710
 Ion Ratio Lower Upper
 172 100
 171 36.0 28.5 42.7
 170 24.3 18.8 28.2

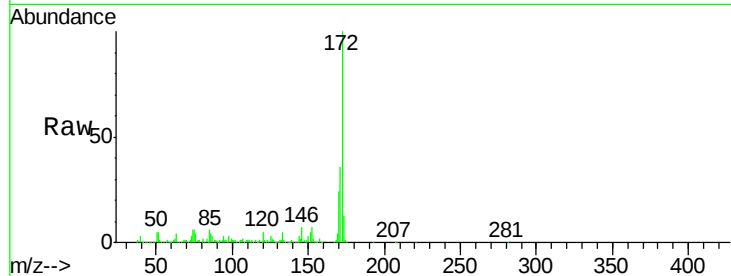

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 16.84 min Scan# 2372
 Delta R.T. -0.01 min
 Lab File: BM010933.D
 Acq: 21 Jul 2017 08:59

Tgt Ion:188 Resp: 1246876
 Ion Ratio Lower Upper
 188 100
 94 6.9 8.7 13.1#
 80 7.7 9.3 13.9#

