
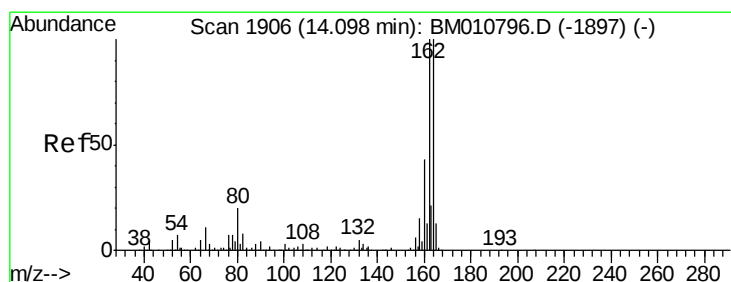
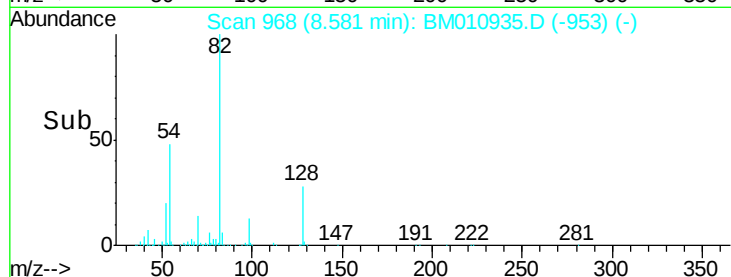
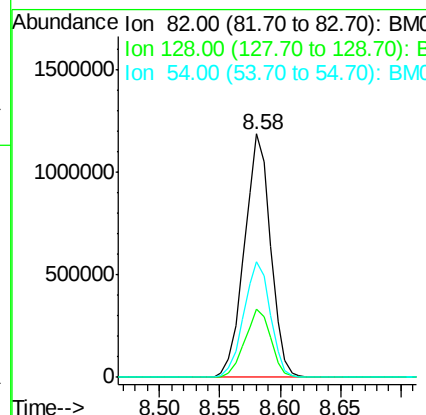


#23
 Nitrobenzene-d5
 Concen: 103.898 ng
 RT: 8.58 min Scan# 968
 Delta R.T. -0.01 min
 Lab File: BM010935.D
 Acq: 21 Jul 2017 10:11

Instrument :
 BNA_M
 ClientSampleId :

Tgt Ion: 82 Resp: 1793652
 Ion Ratio Lower Upper
 82 100
 128 28.3 32.8 49.2#
 54 47.7 40.6 60.8

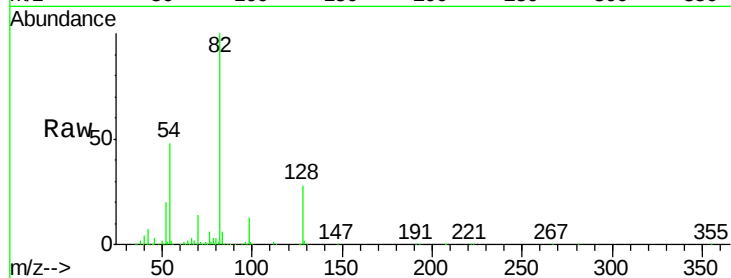

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.09 min Scan# 1904
 Delta R.T. -0.01 min
 Lab File: BM010935.D
 Acq: 21 Jul 2017 10:11

Tgt Ion: 164 Resp: 438672
 Ion Ratio Lower Upper
 164 100
 162 109.0 82.4 123.6
 160 50.9 35.8 53.6

