
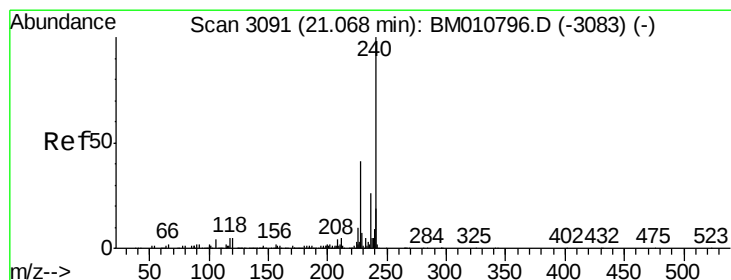
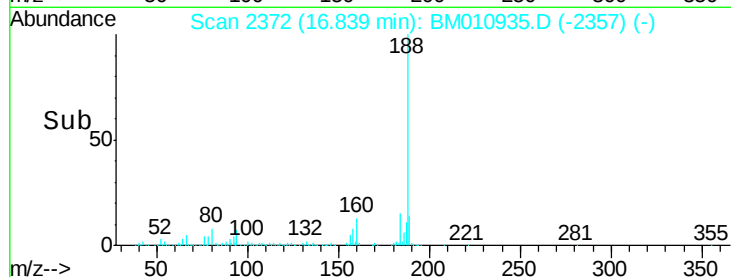
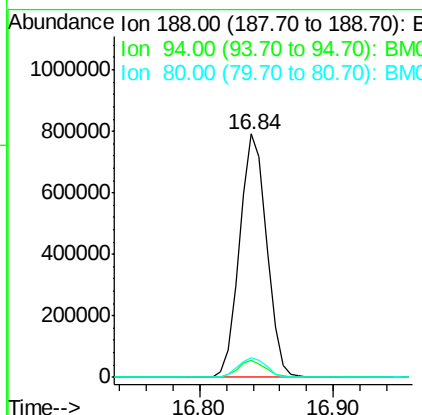


#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.84 min Scan# 2372
Delta R.T. -0.01 min
Lab File: BM010935.D
Acq: 21 Jul 2017 10:11

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:188 Resp: 1108099
Ion Ratio Lower Upper
188 100
94 7.2 8.7 13.1#
80 8.0 9.3 13.9#

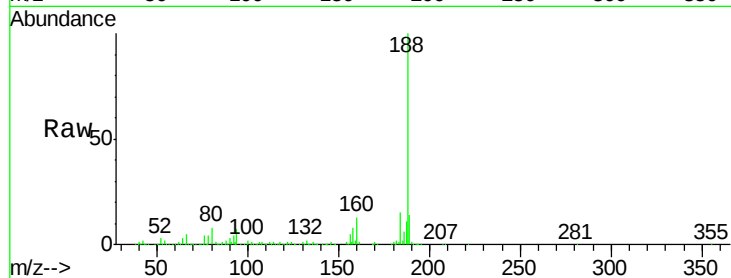

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.06 min Scan# 3089
Delta R.T. -0.01 min
Lab File: BM010935.D
Acq: 21 Jul 2017 10:11

Tgt Ion:240 Resp: 1118963
Ion Ratio Lower Upper
240 100
120 5.2 8.2 12.2#
236 25.6 20.0 30.0

