


Data Path : Z:\HPCHEM1\BNA M\Data\BM072017\
 Data File : BM010905.D
 Acq On : 20 Jul 2017 12:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

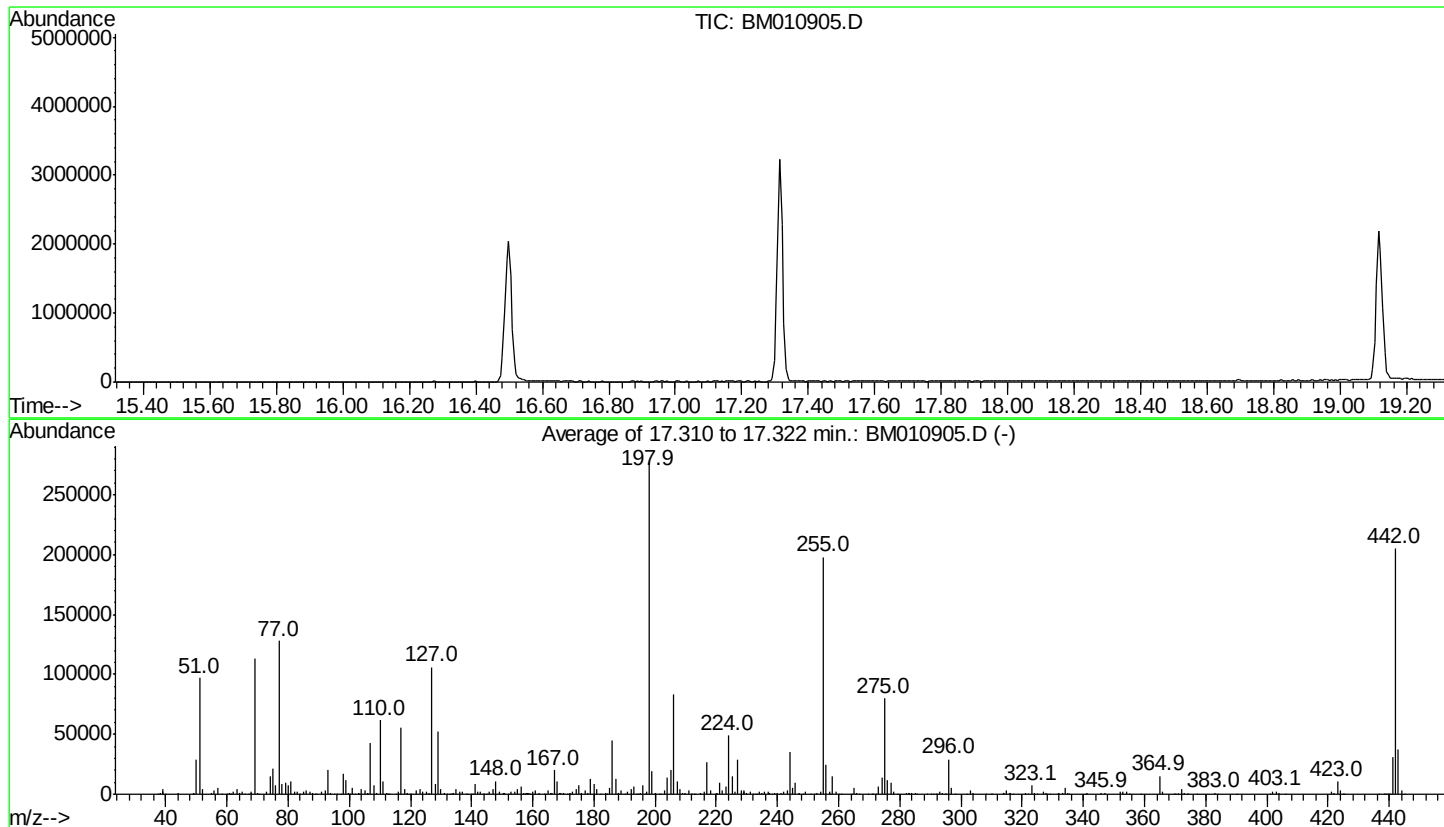

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	97162	PASS
68	69	0.00	2	1.5	1743	PASS
69	198	0.00	100	40.9	113296	PASS
70	69	0.00	2	0.6	676	PASS
127	198	10	80	38.4	106154	PASS
197	198	0.00	2	0.6	1751	PASS
198	198	100	100	100.0	276693	PASS
199	198	5	9	7.0	19314	PASS
275	198	10	60	28.8	79802	PASS
365	198	1	100	5.5	15144	PASS
441	442	0.01	24	15.1	30853	PASS
442	198	50	100	73.9	204608	PASS
443	442	15	24	18.5	37792	PASS