


Data Path : Z:\HPCHEM1\BNA M\Data\BM072017\
 Data File : BM010924.D
 Acq On : 21 Jul 2017 00:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

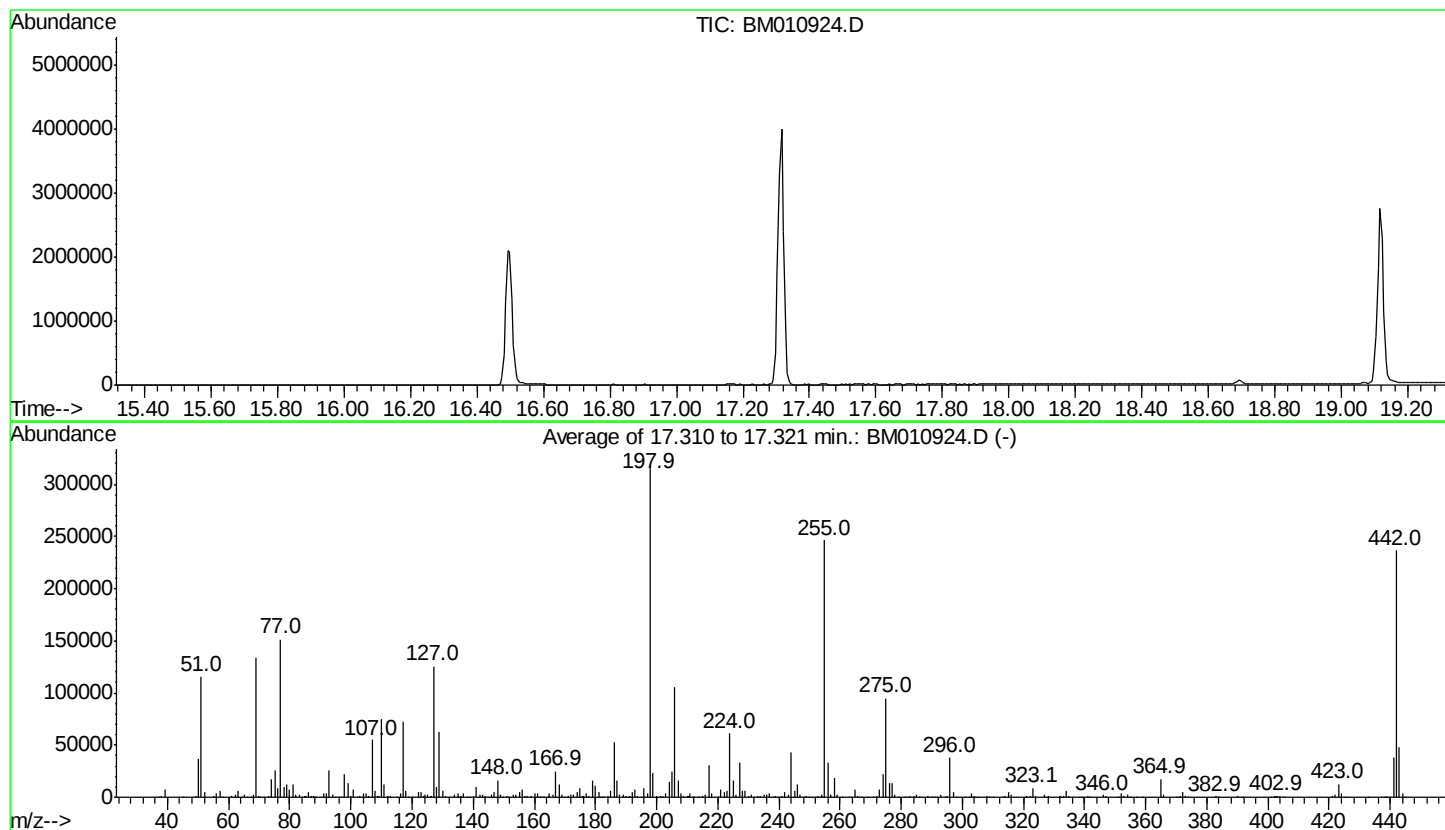

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	115461	PASS
68	69	0.00	2	1.7	2224	PASS
69	198	0.00	100	42.1	133962	PASS
70	69	0.00	2	0.6	809	PASS
127	198	10	80	39.5	125642	PASS
197	198	0.00	2	1.1	3472	PASS
198	198	100	100	100.0	317866	PASS
199	198	5	9	7.2	22987	PASS
275	198	10	60	29.8	94784	PASS
365	198	1	100	5.4	17213	PASS
441	442	0.01	24	15.9	37480	PASS
442	198	50	100	74.4	236458	PASS
443	442	15	24	20.2	47717	PASS