

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
 Data File : BM035875.D
 Acq On : 20 Jul 2022 10:42
 Operator : CG/JU
 Sample : PB145953BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145953BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.046	158	163	169	rVB	120866	154676	1.16%	0.207%
2	5.457	396	403	420	rBV	6881506	9455553	71.09%	12.682%
3	7.063	668	676	690	rBV	6229132	9498286	71.42%	12.739%
4	7.898	811	818	826	rBV	1244335	1912681	14.38%	2.565%
5	9.063	1007	1016	1031	rBV	3729708	5947405	44.72%	7.977%
6	10.704	1286	1295	1303	rBV	1604032	2657347	19.98%	3.564%
7	13.163	1706	1713	1725	rVB	9168358	12854827	96.65%	17.241%
8	14.527	1938	1945	1953	rBV	2130569	3103691	23.34%	4.163%
9	16.015	2190	2198	2219	rBV	5291515	7587049	57.05%	10.176%
10	17.268	2404	2411	2421	rBV	2422231	3222594	24.23%	4.322%
11	19.892	2851	2857	2873	rBV	11518730	13299942	100.00%	17.838%
12	21.439	3116	3120	3130	rBV	1997882	2560292	19.25%	3.434%
13	23.815	3518	3524	3533	rVB	1171013	2305030	17.33%	3.092%




Sum of corrected areas: 74559373

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
Data File : BM035875.D
Acq On : 20 Jul 2022 10:42
Operator : CG/JU
Sample : PB145953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

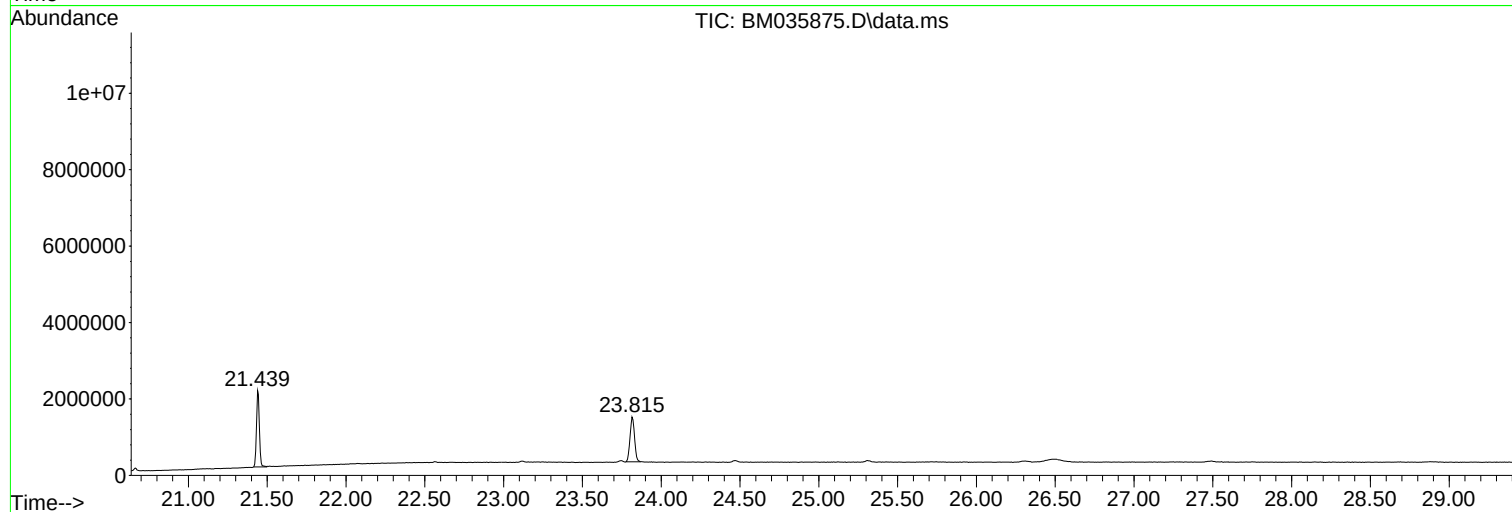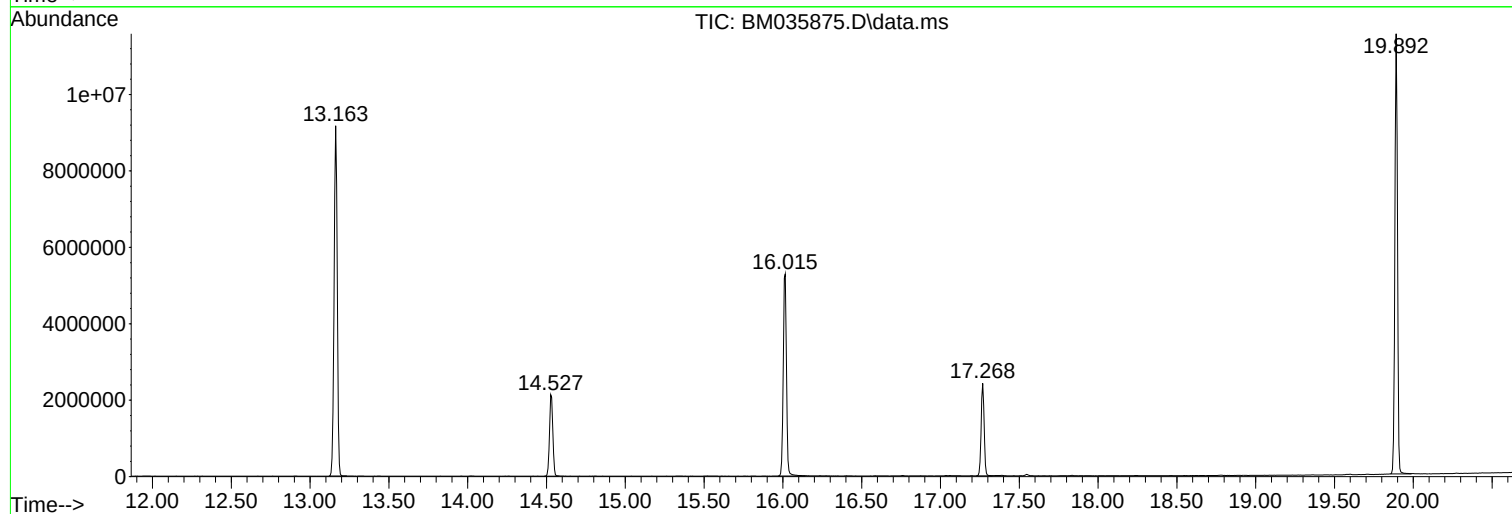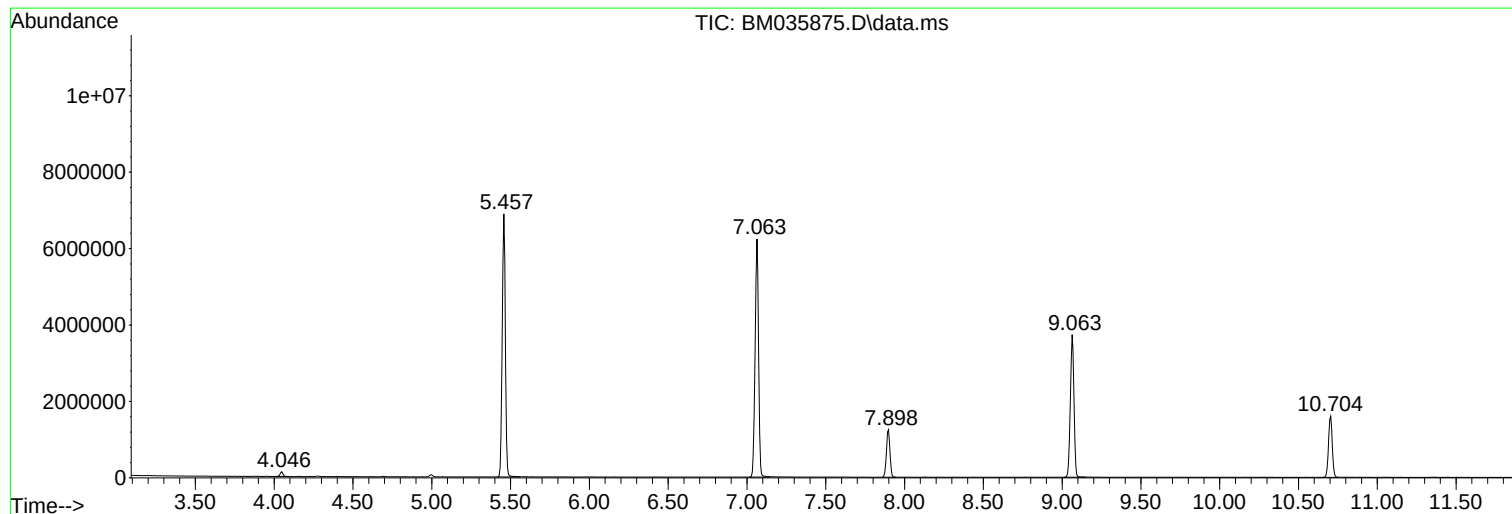

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
Data File : BM035875.D
Acq On : 20 Jul 2022 10:42
Operator : CG/JU
Sample : PB145953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
Data File : BM035875.D
Acq On : 20 Jul 2022 10:42
Operator : CG/JU
Sample : PB145953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------