

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
 Data File : BM035880.D
 Acq On : 20 Jul 2022 14:27
 Operator : CG/JU
 Sample : PB145957BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145957BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.046	159	163	169	rVB	131284	159825	1.13%	0.201%
2	5.458	396	403	416	rBV	7562942	10501555	74.41%	13.193%
3	7.063	667	676	692	rBV	6836326	10589475	75.03%	13.303%
4	7.899	811	818	825	rBV	1328553	2052424	14.54%	2.578%
5	9.063	1008	1016	1032	rBV	4070664	6530695	46.27%	8.204%
6	10.704	1287	1295	1305	rBV	1748817	2844248	20.15%	3.573%
7	13.163	1706	1713	1726	rBV	9969094	14113416	100.00%	17.730%
8	14.533	1938	1946	1958	rBV	2237439	3332922	23.62%	4.187%
9	16.016	2191	2198	2215	rBV	5841182	8180261	57.96%	10.276%
10	17.269	2405	2411	2421	rBV	2412961	3307770	23.44%	4.155%
11	19.898	2852	2858	2869	rBV	10498264	13191351	93.47%	16.572%
12	21.445	3116	3121	3131	rBV	2002891	2532231	17.94%	3.181%
13	23.821	3519	3525	3536	rVB2	1159414	2266262	16.06%	2.847%




Sum of corrected areas: 79602435

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
Data File : BM035880.D
Acq On : 20 Jul 2022 14:27
Operator : CG/JU
Sample : PB145957BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

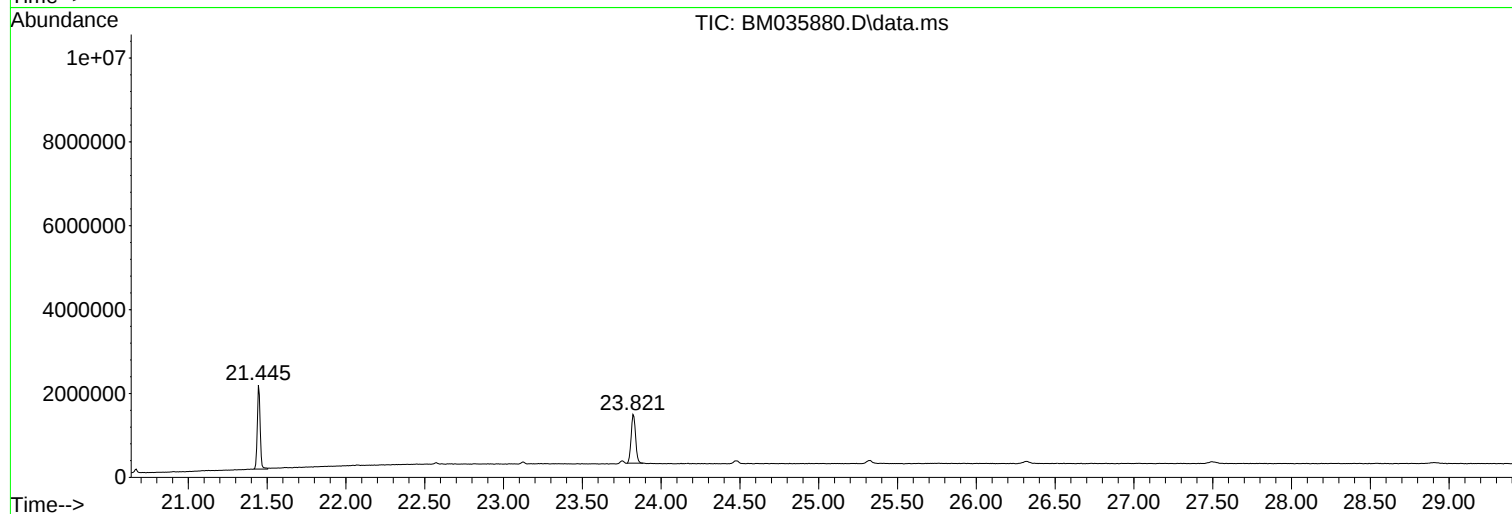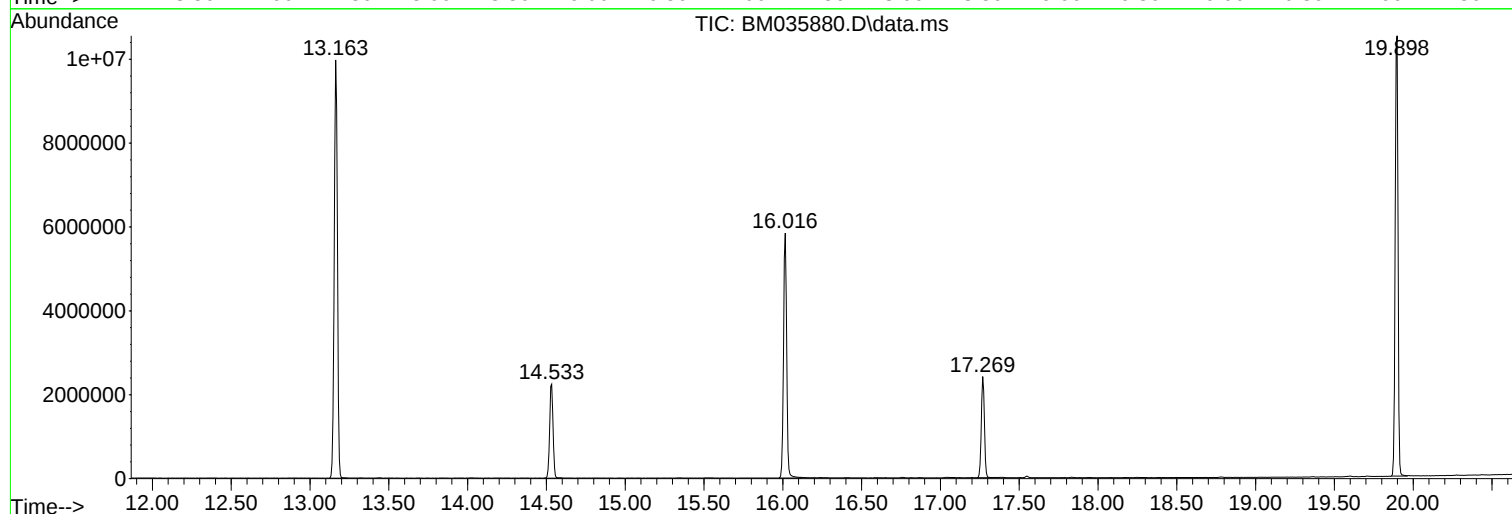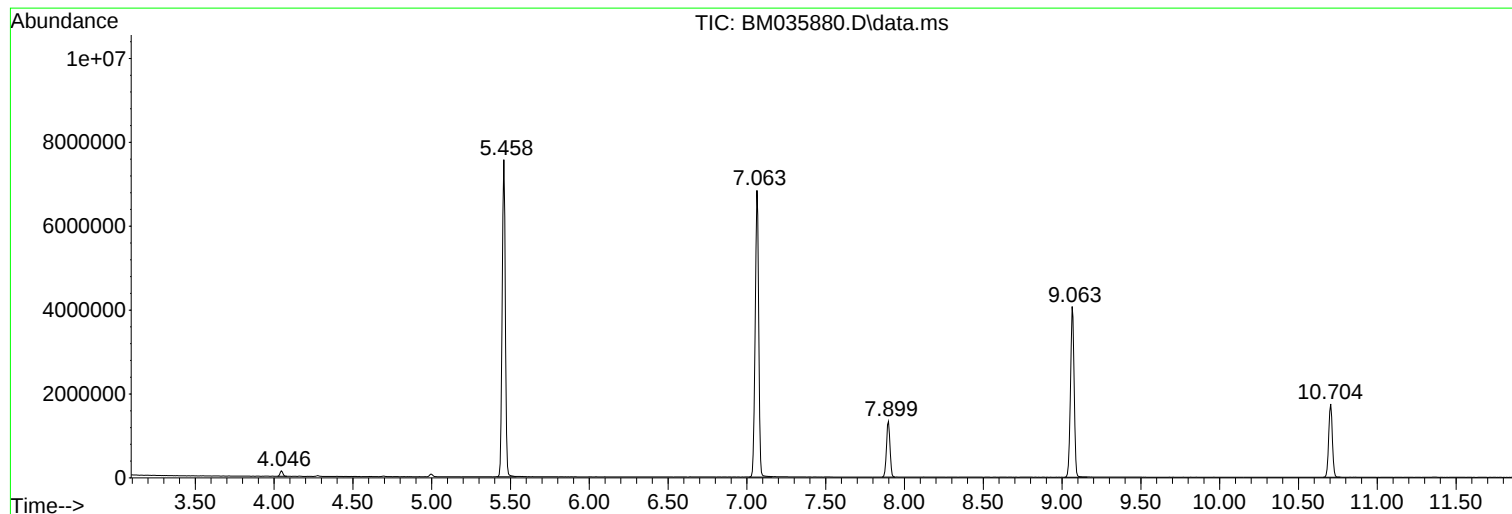

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
Data File : BM035880.D
Acq On : 20 Jul 2022 14:27
Operator : CG/JU
Sample : PB145957BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072022\
Data File : BM035880.D
Acq On : 20 Jul 2022 14:27
Operator : CG/JU
Sample : PB145957BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------