


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072115\
Data File : BM001996.D
Acq On : 21 Jul 2015 21:13
Operator : TP/UM
Sample : DFTPP78
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP78

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Title : SVOA CALIBRATION
Last Update : Wed Jul 22 11:57:37 2015

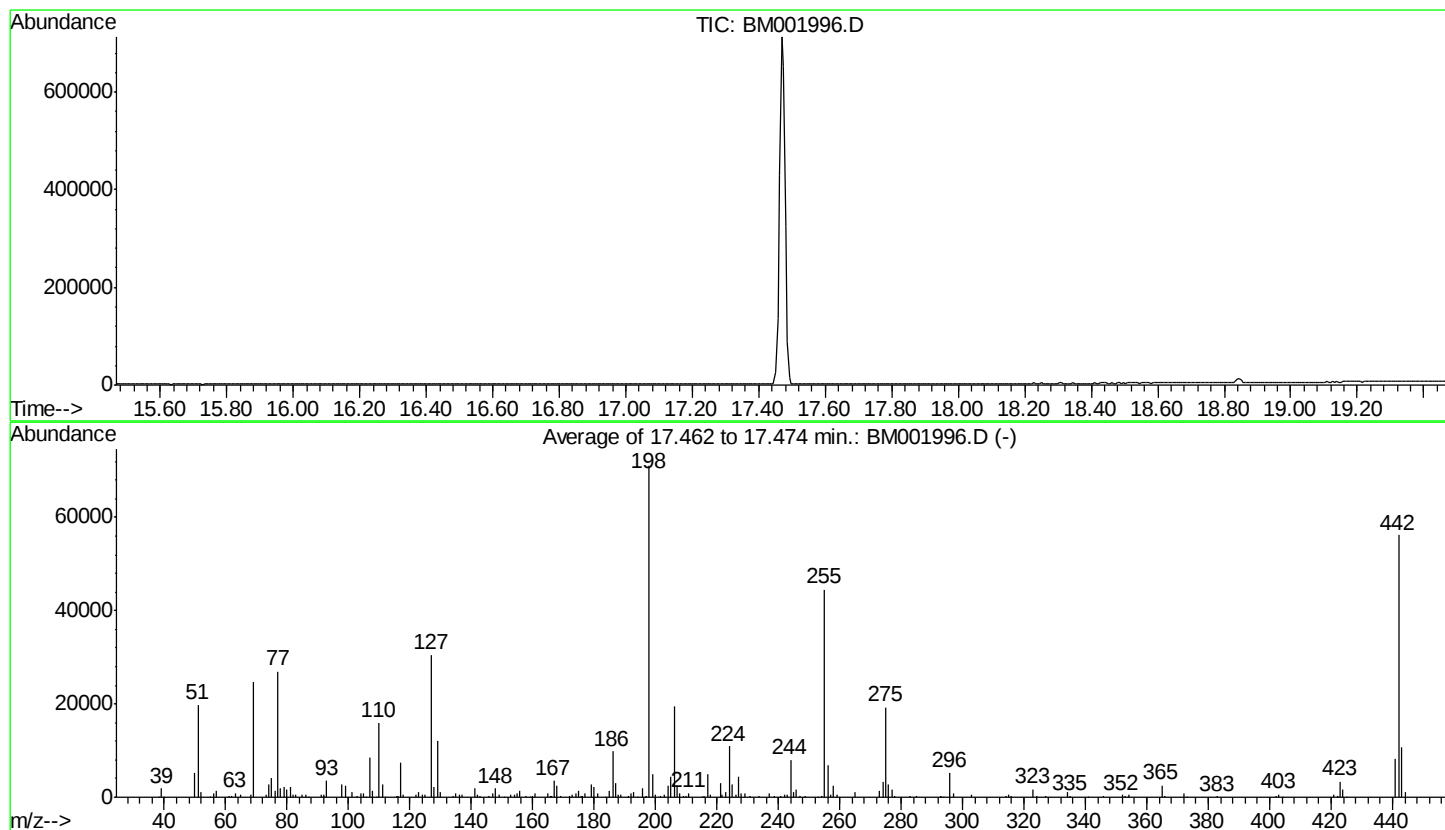

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	19872	PASS
68	69	0.00	2	2.5	631	FAIL*
69	198	0.00	100	34.9	24810	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	30578	PASS
197	198	0.00	2	0.6	413	PASS
198	198	100	100	100.0	71125	PASS
199	198	5	9	7.0	4944	PASS
275	198	10	60	27.2	19362	PASS
365	198	1	100	3.6	2564	PASS
441	443	0.01	100	78.3	8327	PASS
442	198	50	100	79.1	56250	PASS
443	442	15	24	18.9	10631	PASS