

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072116\
 Data File : BM006597.D
 Acq On : 21 Jul 2016 21:00
 Operator : UM/SJ
 Sample : H4078-08MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YS2MSD

Quant Time: Jul 22 01:57:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 22 01:56:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	134175	20.00	ng/ul	0.00
7) Naphthalene-d8	10.39	136	587921	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.26	164	335610	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.02	188	774339	20.00	ng/ul	0.00
29) Chrysene-d12	21.22	240	900960	20.00	ng/ul	0.00
34) Perylene-d12	23.41	264	941163	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.13	96	5251	1.58	ng/uL	0.00
3) Phenol-d5	6.79	99	209118	18.32	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.95	67	141961	20.08	ng/ul	0.00
5) 2-Chlorophenol-d4	7.15	132	170866	18.73	ng/ul	0.00
6) 4-Methylphenol-d8	8.32	113	126832	14.33	ng/ul	0.00
8) Nitrobenzene-d5	8.76	128	84980	19.10	ng/ul	0.00
9) 2-Nitrophenol-d4	9.48	143	89970	19.01	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.02	165	163246	18.25	ng/ul	0.00
12) 4-Chloroaniline-d4	10.53	131	196792	19.98	ng/ul	0.00
16) Dimethylphthalate-d6	13.67	166	525059	19.95	ng/ul	0.00
17) Acenaphthylene-d8	13.95	160	670983	19.98	ng/ul	0.00
20) 4-Nitrophenol-d4	14.48	143	55770	12.20	ng/ul	0.00
21) Fluorene-d10	15.26	176	478056	20.31	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.40	200	52952	13.17	ng/ul	0.00
26) Anthracene-d10	17.11	188	724096	19.69	ng/ul	0.00
30) Pyrene-d10	19.42	212	833607	20.31	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.27	264	875881	20.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) Acenaphthene	14.33	153	451140	19.51	ng/ul	94
25) Phenanthrene	17.06	178	291439	6.69	ng/ul	97
27) Anthracene	17.14	178	63101	1.41	ng/ul	98
28) Fluoranthene	19.08	202	518772	10.14	ng/ul	98
31) Pyrene	19.44	202	1439693	26.39	ng/ul	97
32) Benzo(a)anthracene	21.20	228	245422	4.49	ng/ul	98
33) Chrysene	21.25	228	227801	4.52	ng/ul	99
35) Benzo(b)fluoranthene	22.76	252	318415	5.64	ng/ul	99
36) Benzo(k)fluoranthene	22.76	252	318415	5.84	ng/ul	100
38) Benzo(a)pyrene	23.31	252	221622	4.04	ng/ul	98
39) Indeno(1,2,3-cd)pyrene	25.60	276	155228	2.44	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072116\
Data File : BM006597.D
Acq On : 21 Jul 2016 21:00
Operator : UM/SJ
Sample : H4078-08MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9YS2MSD

Quant Time: Jul 22 01:57:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 22 01:56:00 2016
Response via : Initial Calibration

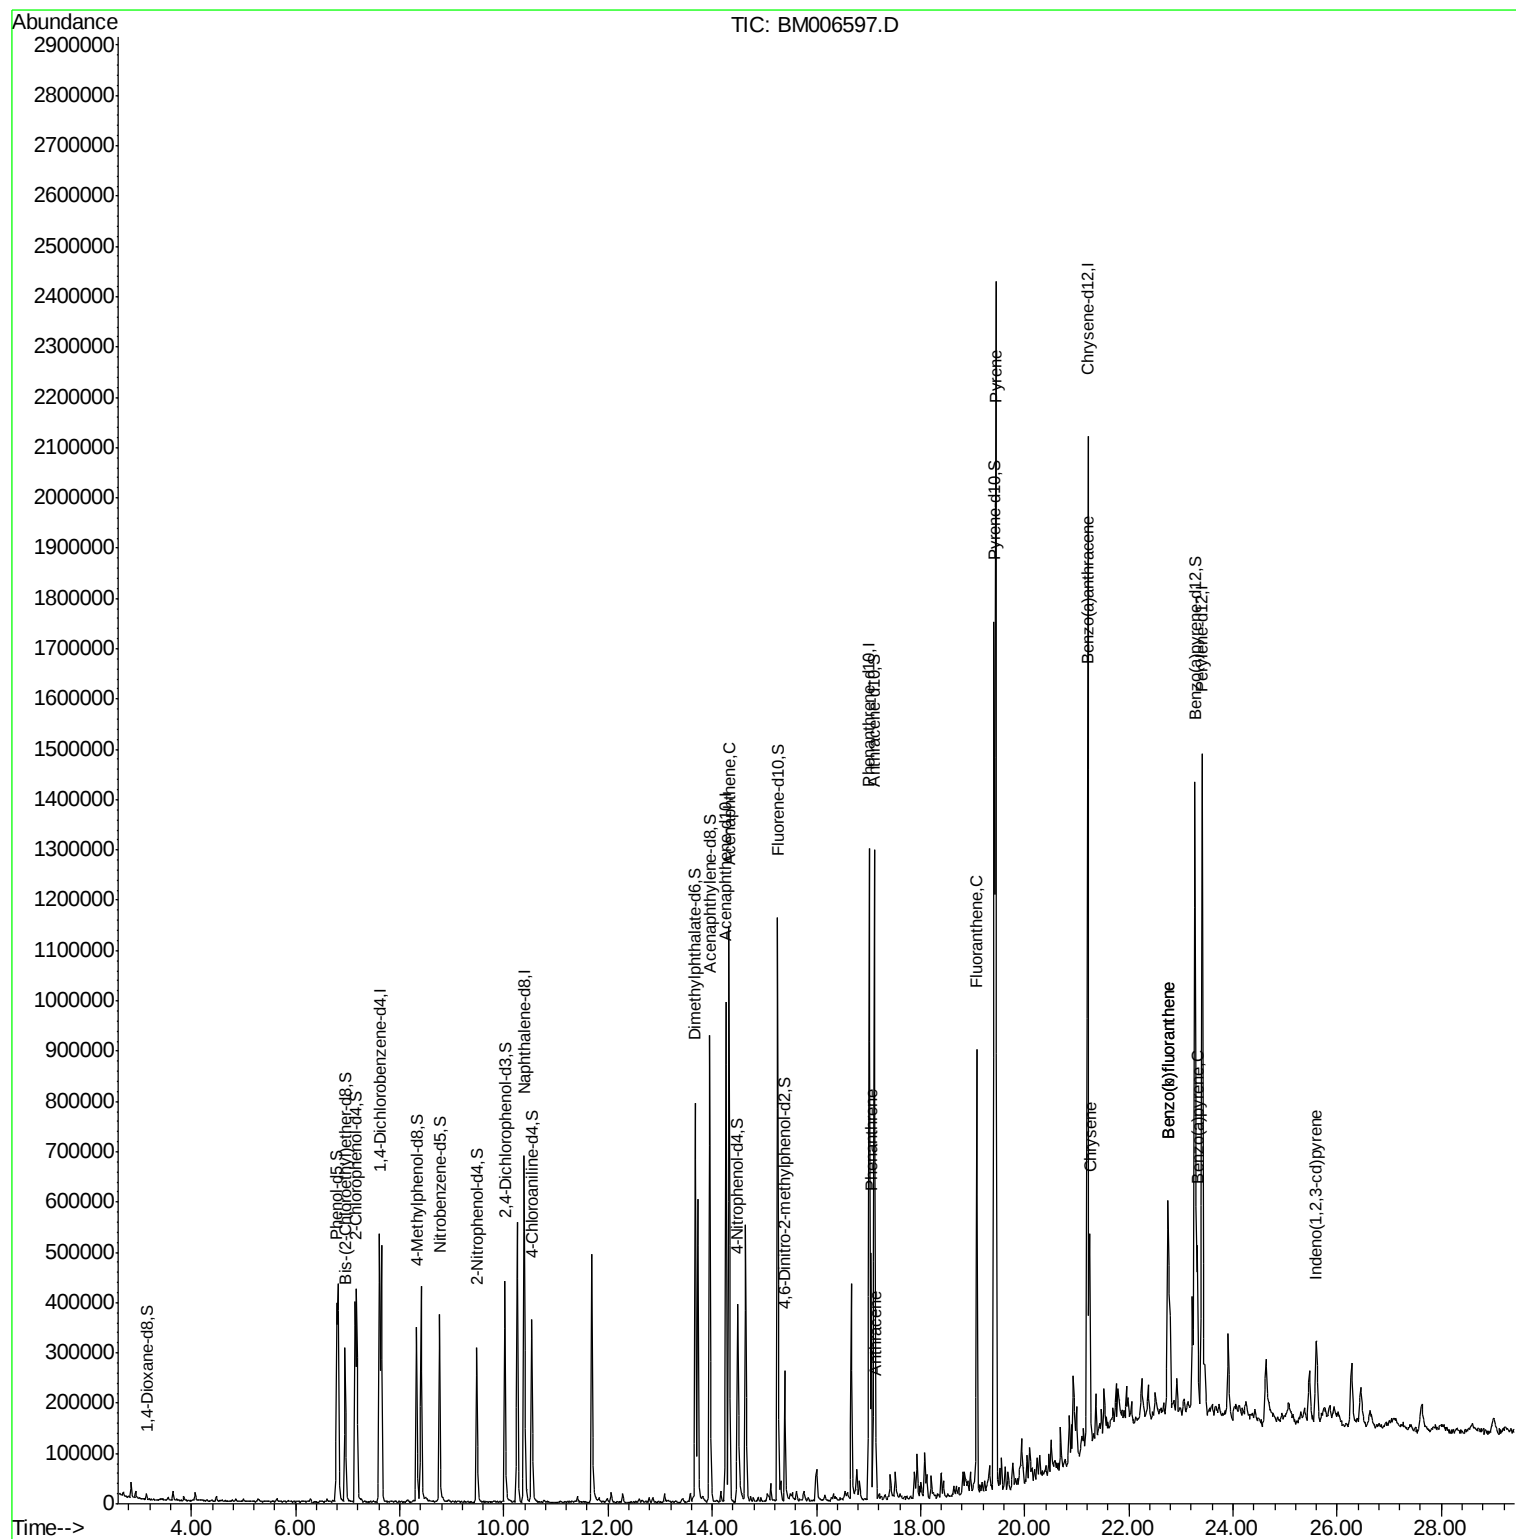

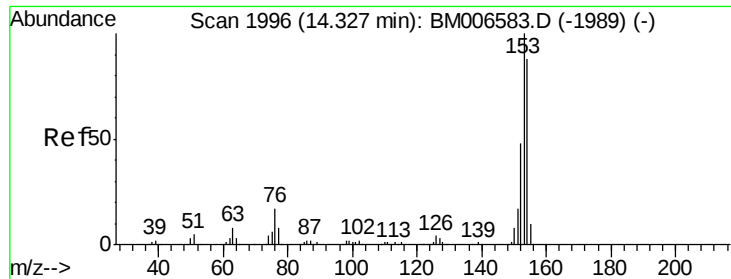

#19

Acenaphthene

Concen: 19.51 ng/ul

RT: 14.33 min Scan# 1996

Delta R.T. 0.00 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00

Instrument :

BNA_M

ClientSampleId :

D9YS2MSD


Tgt Ion:153 Resp: 451140

Ion Ratio Lower Upper

153 100

152 48.6 36.5 54.7




154 90.5 67.3 100.9

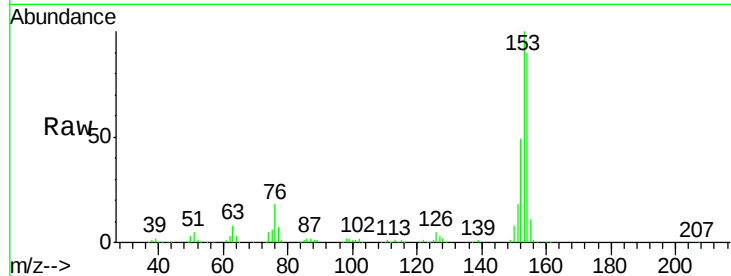

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

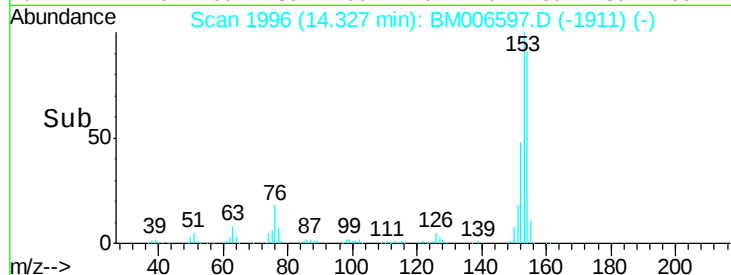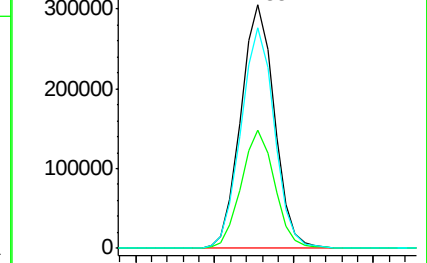

#25

Phenanthrene

Concen: 6.69 ng/ul

RT: 17.06 min Scan# 2460

Delta R.T. 0.00 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00


Tgt Ion:178 Resp: 291439

Ion Ratio Lower Upper

178 100

179 16.3 11.8 17.8



176 19.5 14.8 22.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

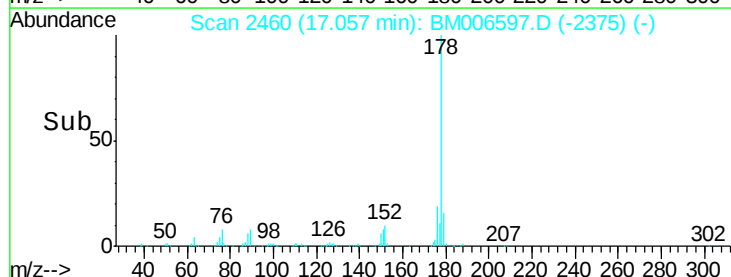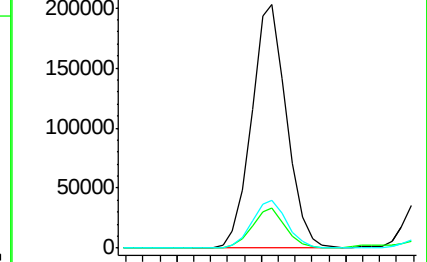

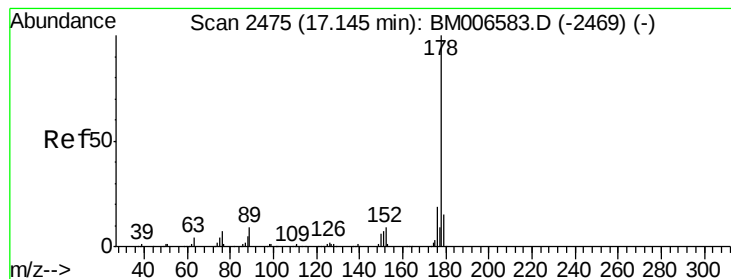

#27

Anthracene

Concen: 1.41 ng/ul

RT: 17.14 min Scan# 2475

Delta R.T. 0.00 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00

Instrument :

BNA_M

ClientSampleId :

D9YS2MSD


Tgt Ion:178 Resp: 63101

Ion Ratio Lower Upper

178 100

179 15.6 12.9 19.3




176 18.6 15.6 23.4



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

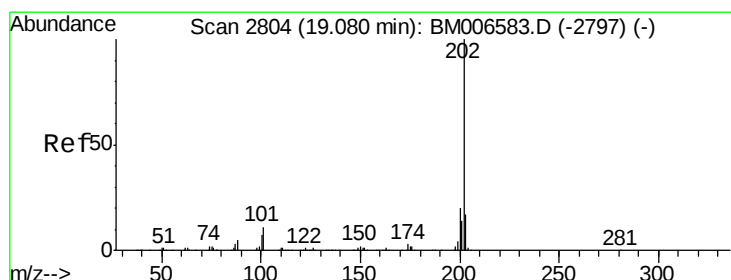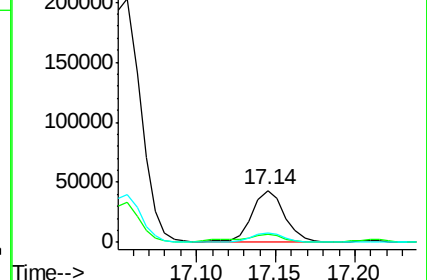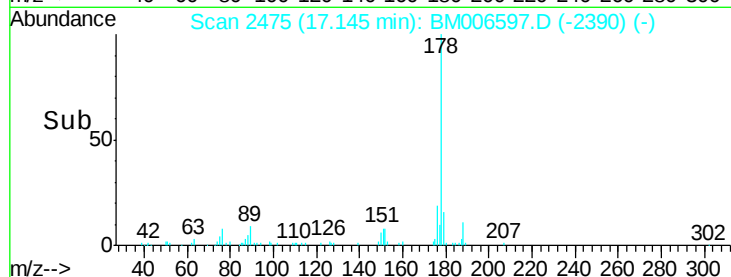

#28

Fluoranthene

Concen: 10.14 ng/ul

RT: 19.08 min Scan# 2804

Delta R.T. 0.00 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00


Tgt Ion:202 Resp: 518772

Ion Ratio Lower Upper

202 100

101 10.9 8.9 13.3



100 7.7 7.0 10.4




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

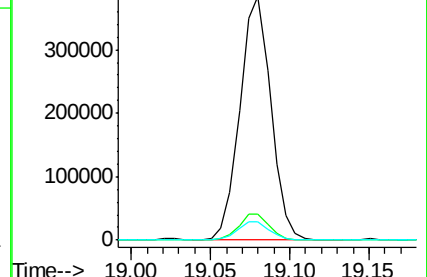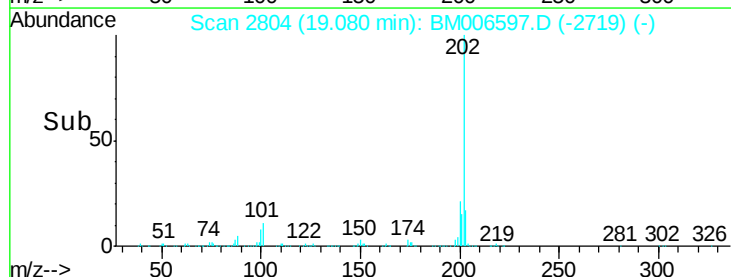


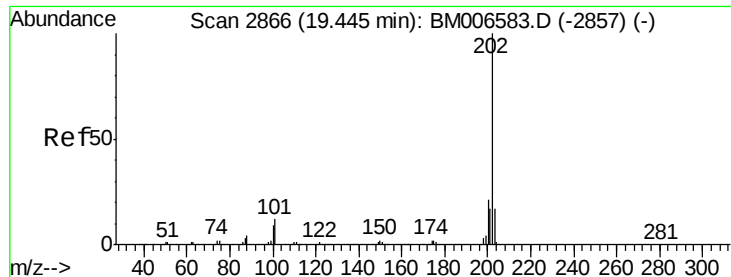




#31
 Pyrene
 Concen: 26.39 ng/ul
 RT: 19.44 min Scan# 2866
 Delta R.T. 0.00 min
 Lab File: BM006597.D
 Acq: 21 Jul 2016 21:00

Instrument :
 BNA_M
 ClientSampleId :
 D9YS2MSD

Tgt Ion:202 Resp: 1439693
 Ion Ratio Lower Upper
 202 100
 101 12.4 9.8 14.8
 100 9.6 9.3 13.9




Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

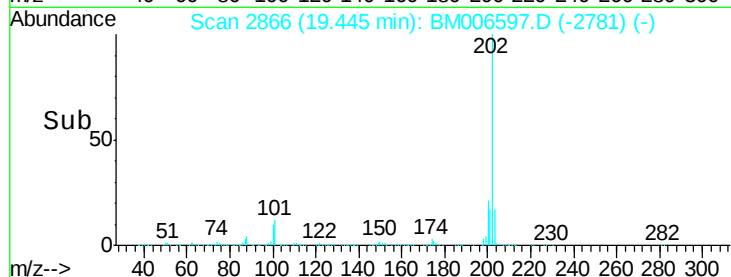
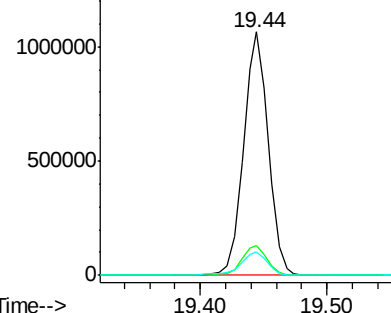



#32
 Benzo(a)anthracene
 Concen: 4.49 ng/ul
 RT: 21.20 min Scan# 3164
 Delta R.T. 0.00 min
 Lab File: BM006597.D
 Acq: 21 Jul 2016 21:00

Tgt Ion:228 Resp: 245422
 Ion Ratio Lower Upper
 228 100
 229 19.9 16.6 25.0
 226 27.2 21.0 31.4



Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 229.00 (228.70 to 229.70): E
 Ion 226.00 (225.70 to 226.70): E

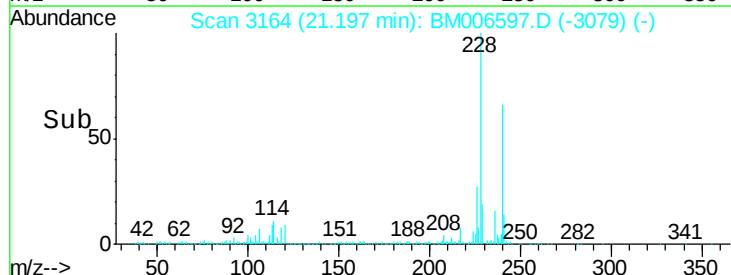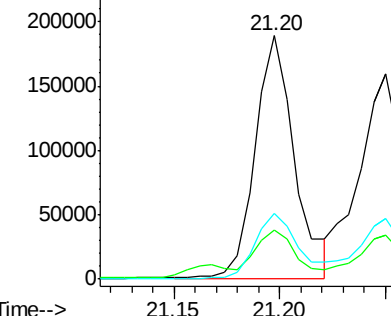

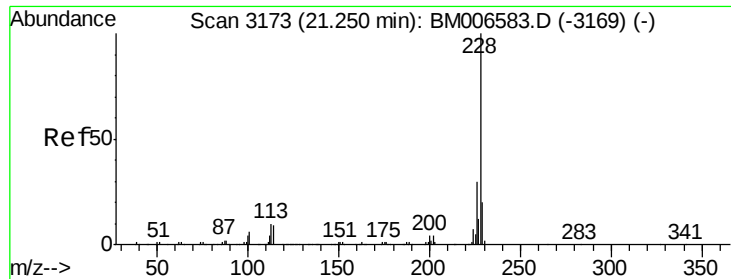

#33

Chrysene

Concen: 4.52 ng/ul

RT: 21.25 min Scan# 3173

Delta R.T. 0.00 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00

Instrument :

BNA_M

ClientSampleId :

D9YS2MSD


Tgt Ion:228 Resp: 227801

Ion Ratio Lower Upper

228 100

226 29.5 23.4 35.2




229 21.2 16.2 24.2



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

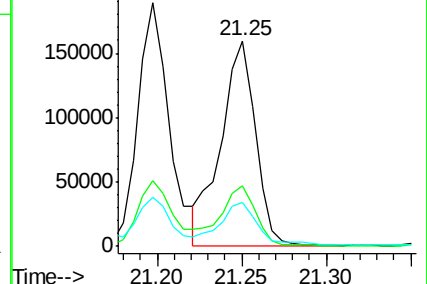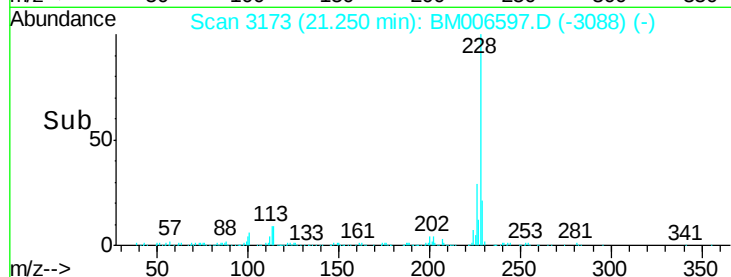

#35

Benzo(b)fluoranthene

Concen: 5.64 ng/ul

RT: 22.76 min Scan# 3429

Delta R.T. 0.00 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00


Tgt Ion:252 Resp: 318415

Ion Ratio Lower Upper

252 100

253 22.2 18.1 27.1



125 9.4 7.6 11.4




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



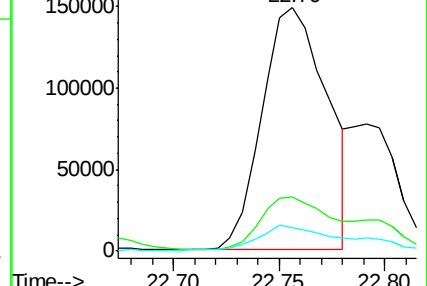
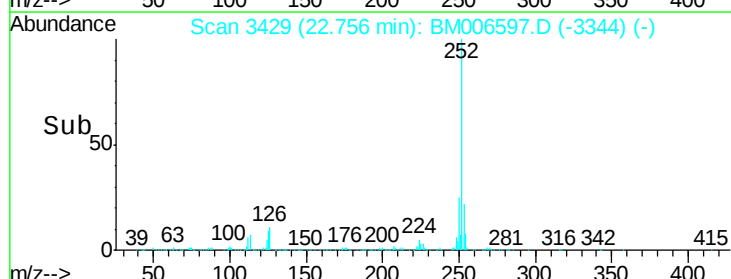


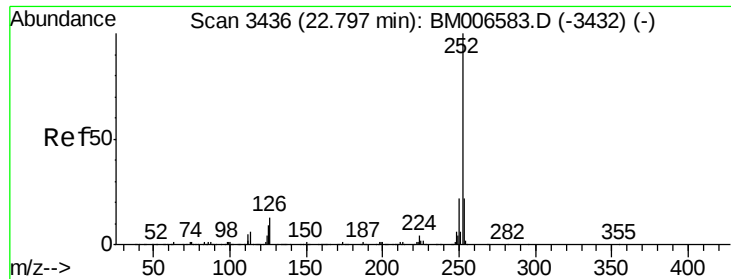

#36
Benzo(k)fluoranthene
Concen: 5.84 ng/ul
RT: 22.76 min Scan# 3429
Delta R.T. -0.04 min
Lab File: BM006597.D
Acq: 21 Jul 2016 21:00




Instrument :
BNA_M
ClientSampleId :
D9YS2MSD


Tgt Ion:252 Resp: 318415
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.8
125 9.4 7.7 11.5

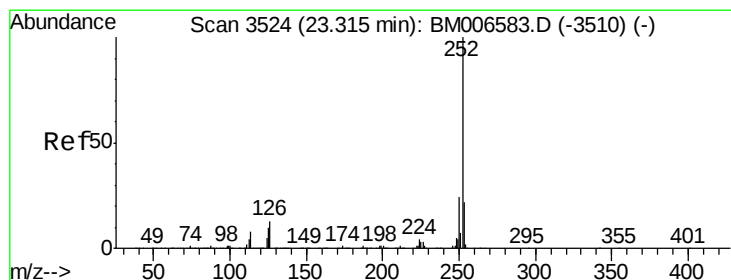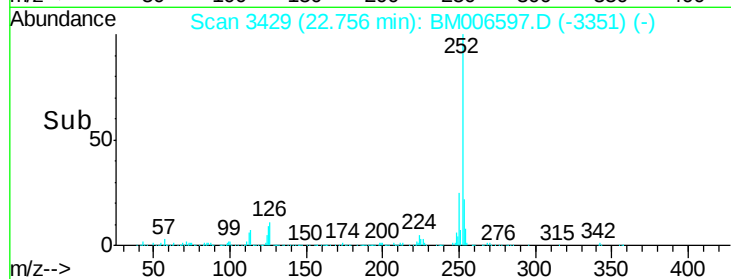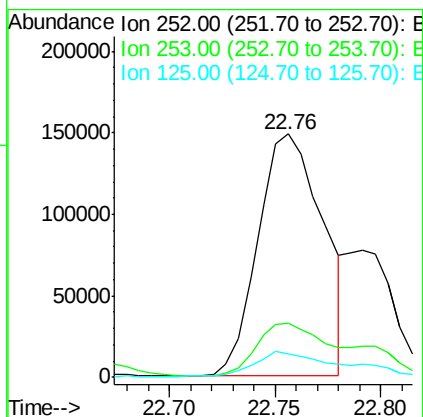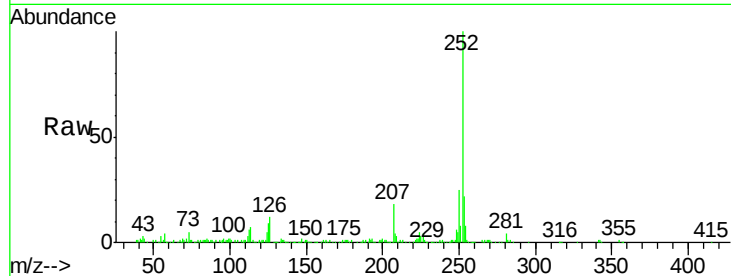

#38
Benzo(a)pyrene
Concen: 4.04 ng/ul
RT: 23.31 min Scan# 3524
Delta R.T. 0.00 min
Lab File: BM006597.D
Acq: 21 Jul 2016 21:00

Tgt Ion:252 Resp: 221622
Ion Ratio Lower Upper
252 100
253 22.7 17.4 26.0
125 9.9 8.2 12.2

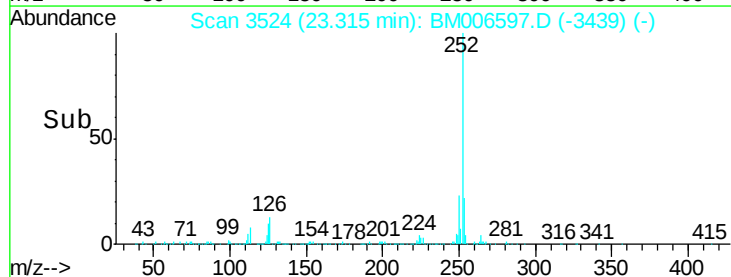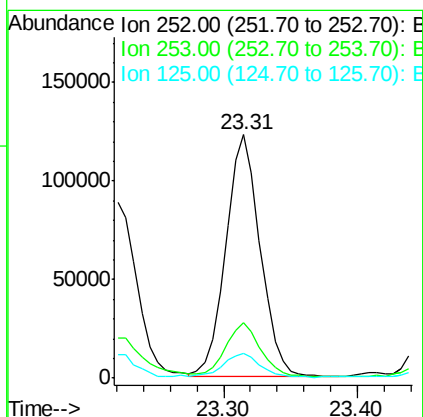

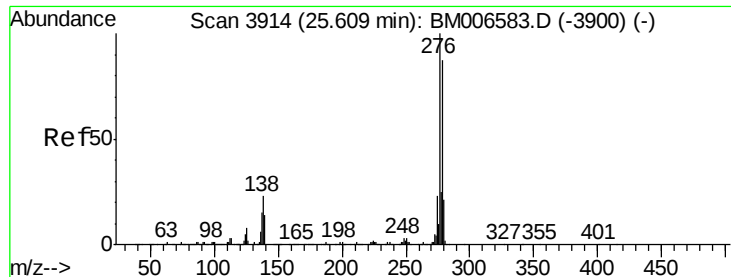

#39

Indeno(1,2,3-cd)pyrene

Concen: 2.44 ng/ul

RT: 25.60 min Scan# 3913

Delta R.T. -0.01 min

Lab File: BM006597.D

Acq: 21 Jul 2016 21:00

Instrument :

BNA_M

ClientSampleId :

D9YS2MSD


Tgt Ion: 276 Resp: 155228

Ion Ratio Lower Upper

276 100

138 18.6 15.8 23.6

277 24.0 19.0 28.6

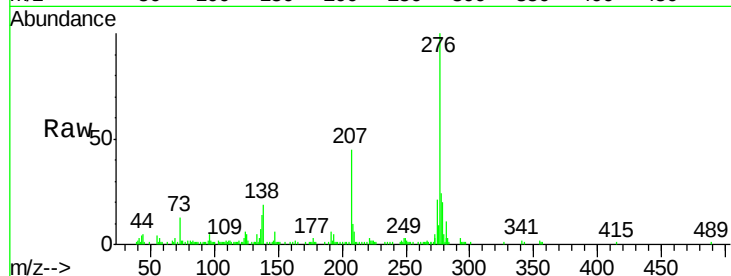

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

