

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072116\
 Data File : BM006598.D
 Acq On : 21 Jul 2016 21:36
 Operator : UM/SJ
 Sample : H4077-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YR5

Manual Integrations

umangi
 7/22/2016 6:24:31 PM

Quant Time: Jul 22 02:33:15 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 22 01:56:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	155515	20.00	ng/ul	0.00
7) Naphthalene-d8	10.39	136	691903	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.26	164	404339	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.02	188	919879m	20.00	ng/ul	0.00
29) Chrysene-d12	21.22	240	1095899	20.00	ng/ul	0.00
34) Perylene-d12	23.41	264	1143216	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.13	96	5267	1.37	ng/uL	0.00
3) Phenol-d5	6.79	99	196680	14.87	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.95	67	137833	16.82	ng/ul	0.00
5) 2-Chlorophenol-d4	7.15	132	162298	15.35	ng/ul	0.00
6) 4-Methylphenol-d8	8.32	113	124638	12.15	ng/ul	0.00
8) Nitrobenzene-d5	8.77	128	83162	15.88	ng/ul	0.00
9) 2-Nitrophenol-d4	9.48	143	87847	15.77	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.02	165	158300	15.04	ng/ul	0.00
12) 4-Chloroaniline-d4	10.53	131	185401	15.99	ng/ul	0.00
16) Dimethylphthalate-d6	13.67	166	533612	16.83	ng/ul	0.00
17) Acenaphthylene-d8	13.95	160	671373	16.59	ng/ul	0.00
20) 4-Nitrophenol-d4	14.49	143	65527	11.90	ng/ul	0.00
21) Fluorene-d10	15.26	176	484775	17.10	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.40	200	53454m	11.20	ng/ul	0.00
26) Anthracene-d10	17.11	188	727367	16.65	ng/ul	0.00
30) Pyrene-d10	19.42	212	861041	17.24	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.27	264	897729	17.07	ng/ul	0.00

Target Compounds

						Ovalue
25) Phenanthrene	17.06	178	62337m	1.20	ng/ul	
28) Fluoranthene	19.08	202	113140	1.86	ng/ul	97
31) Pyrene	19.44	202	103904	1.57	ng/ul	98
32) Benzo(a)anthracene	21.20	228	71531	1.08	ng/ul	95
33) Chrysene	21.25	228	82530	1.35	ng/ul	98
35) Benzo(b)fluoranthene	22.76	252	115853	1.69	ng/ul	98
38) Benzo(a)pyrene	23.31	252	78002	1.17	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM072116\
Data File : BM006598.D
Acq On : 21 Jul 2016 21:36
Operator : UM/SJ
Sample : H4077-11
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9YR5

Manual Integrations

umangi
7/22/2016 6:24:31 PM

Quant Time: Jul 22 02:33:15 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 22 01:56:00 2016
Response via : Initial Calibration

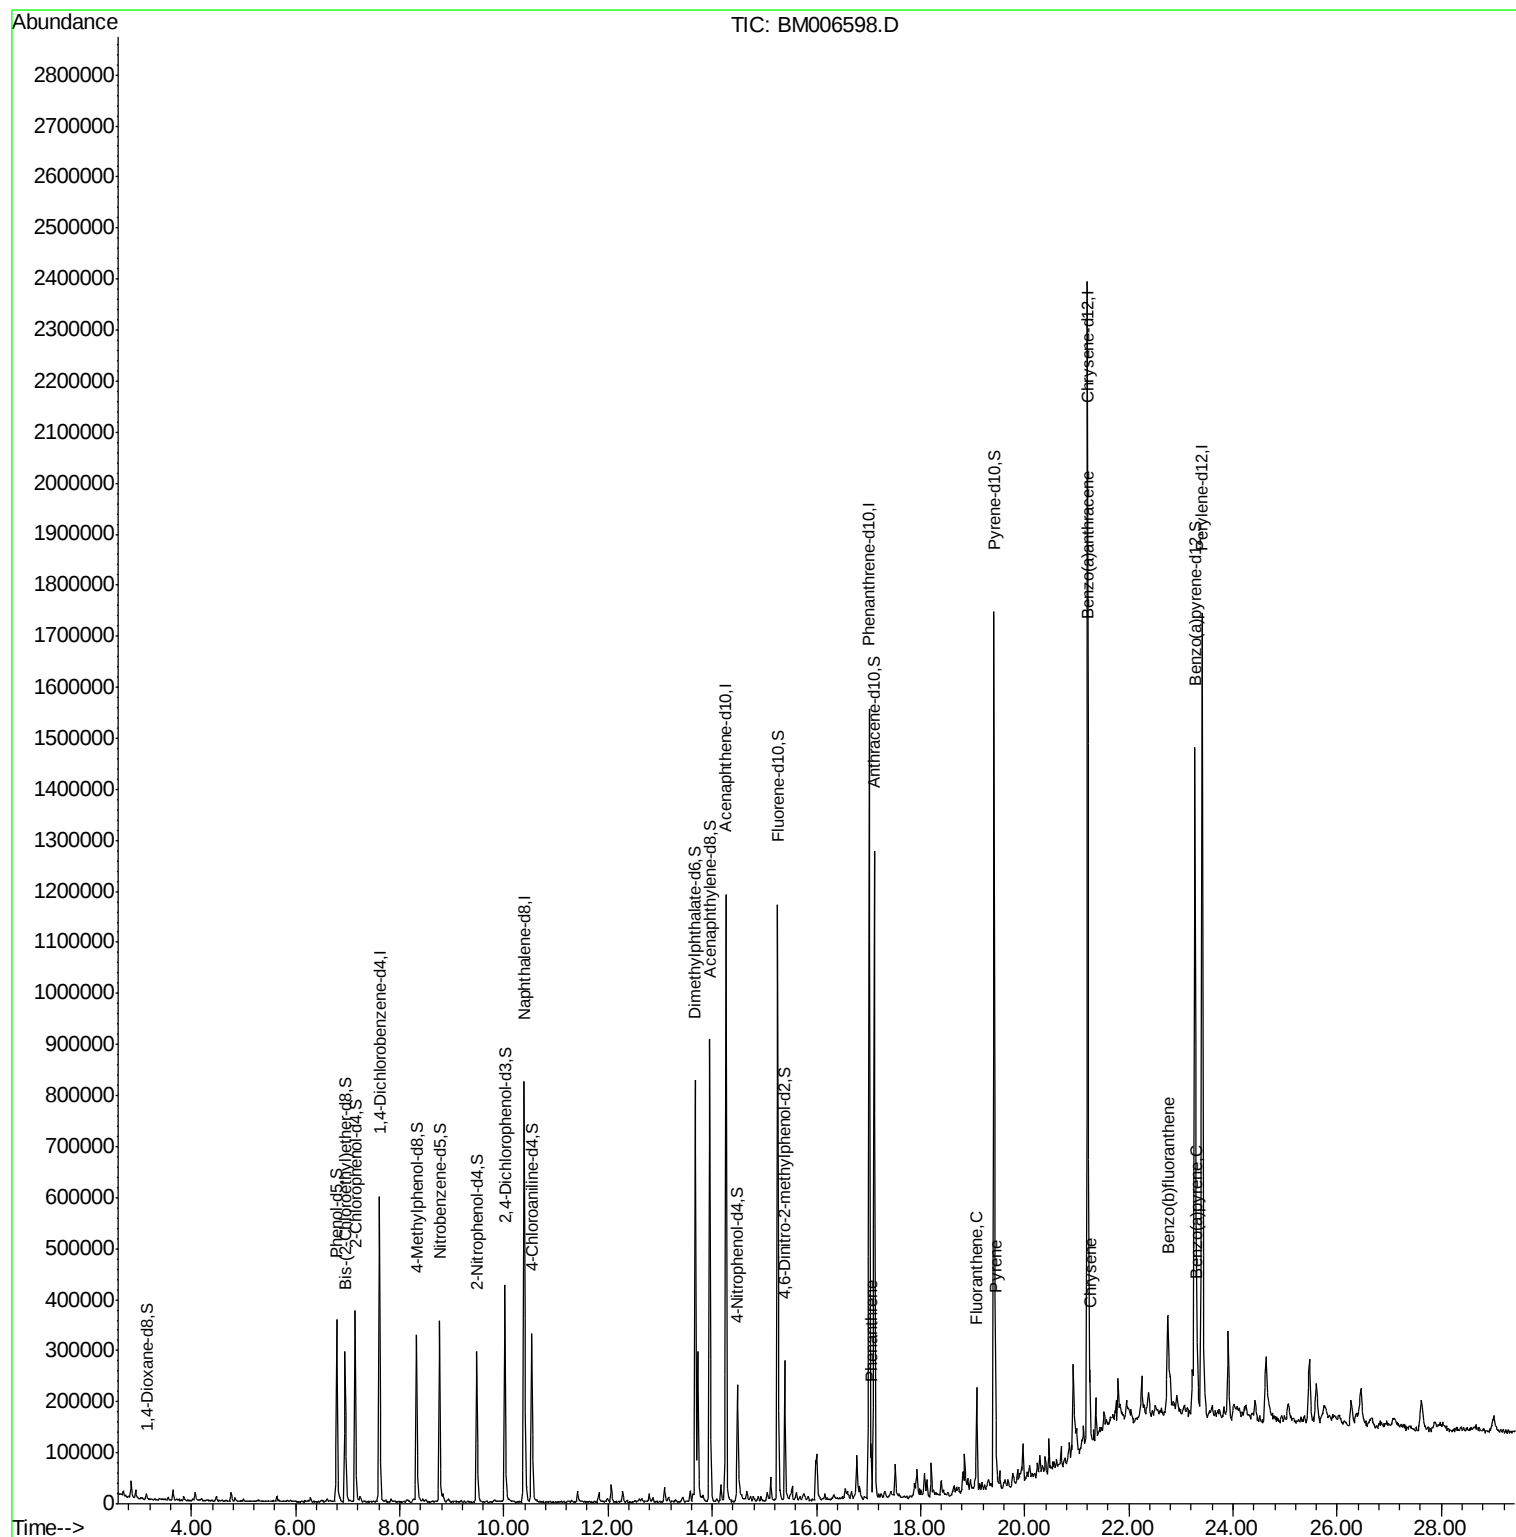

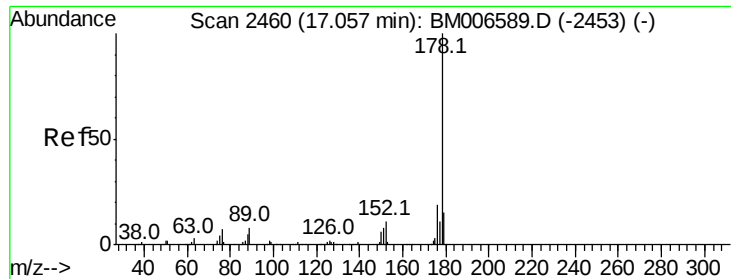

#25

Phenanthrene

Concen: 1.20 ng/ul

RT: 17.06 min Scan# 2460

Delta R.T. 0.00 min

Lab File: BM006598.D

Acq: 21 Jul 2016 21:36

Instrument :

BNA_M

ClientSampleId :

D9YR5

Tot Ion:178 Resp: 62337

Ion Ratio Lower Upper

178 100


179 15.3 11.8 17.8

176 18.6 14.8 22.2

Manual Integrations

umangi




7/22/2016 6:24:31 PM

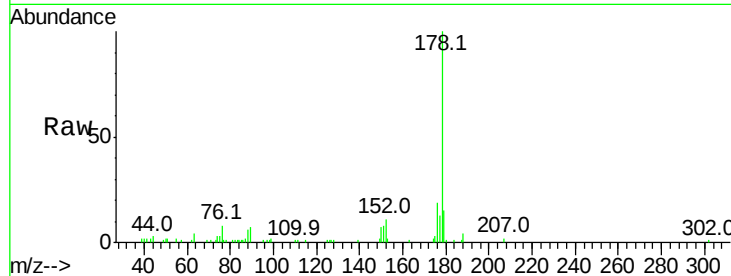

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

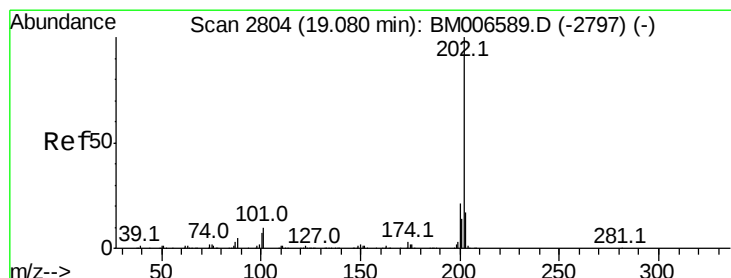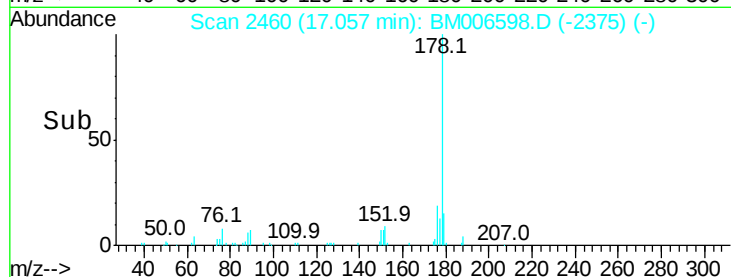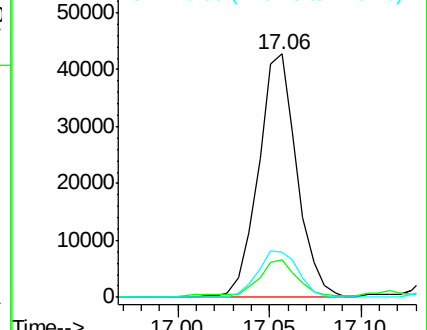

#28

Fluoranthene

Concen: 1.86 ng/ul

RT: 19.08 min Scan# 2804

Delta R.T. 0.00 min

Lab File: BM006598.D

Acq: 21 Jul 2016 21:36


Tgt Ion:202 Resp: 113140

Ion Ratio Lower Upper

202 100

101 10.6 8.9 13.3



100 7.2 7.0 10.4

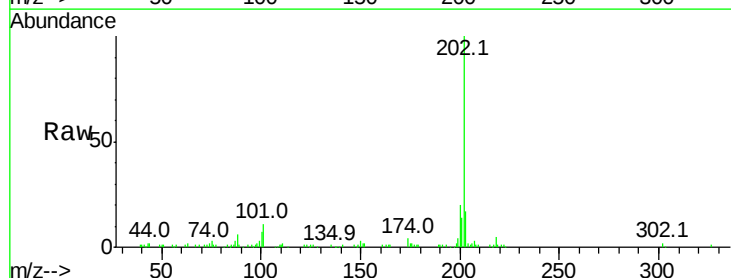


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

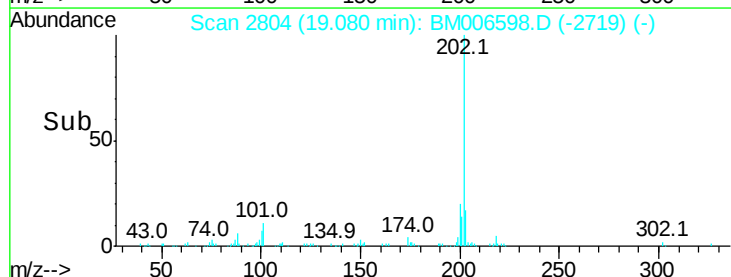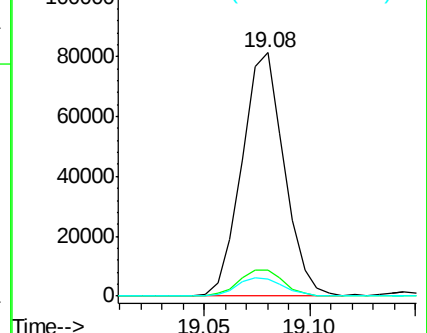

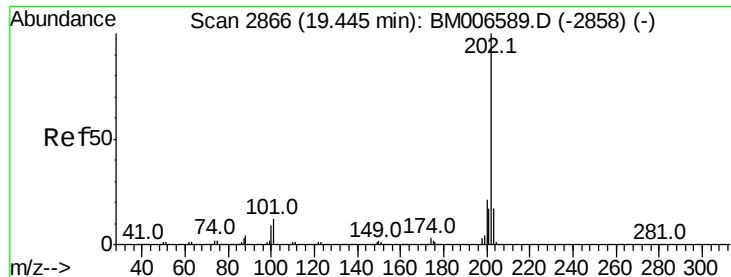





#31
Pvrene
Concen: 1.57 ng/ul
RT: 19.44 min Scan# 2866
Delta R.T. 0.00 min
Lab File: BM006598.D
Acq: 21 Jul 2016 21:36

Instrument :
BNA_M
ClientSampleId :
D9YR5

Tot Ion:	202	Resp:	103904
Ion Ratio	Lower	Upper	
202	100		
101	12.9	9.8	14.8
100	10.4	9.3	13.9




Manual Integrations


umangi
7/22/2016 6:24:31 PM

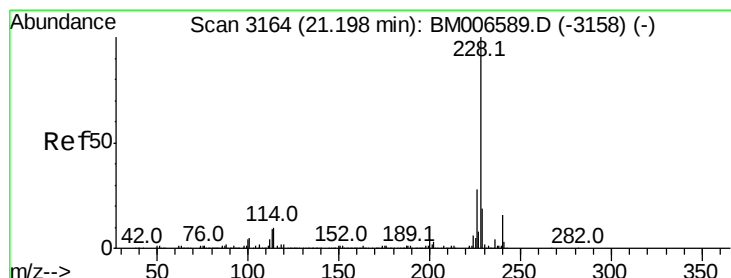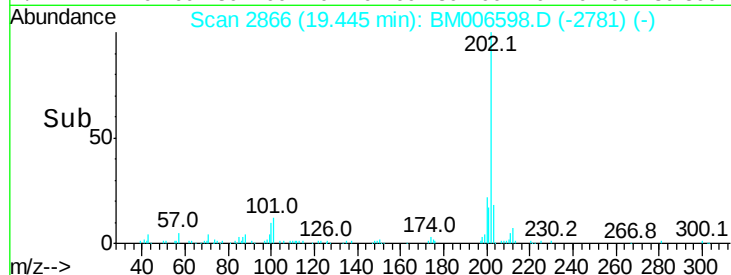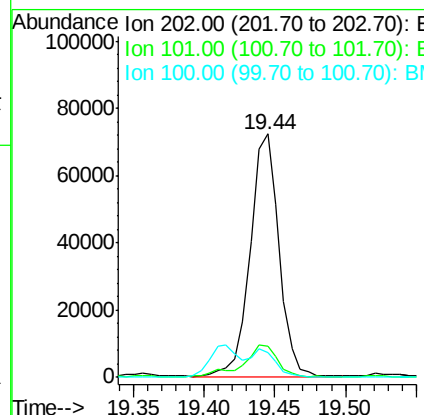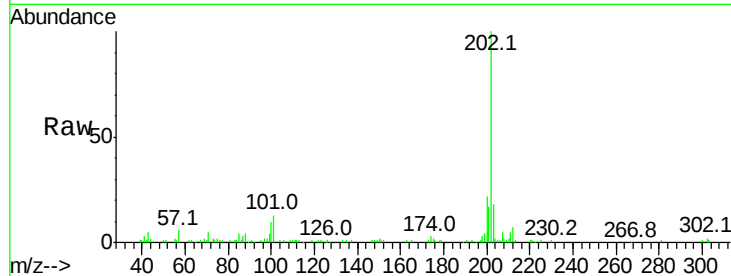

#32
Benzo(a)anthracene
Concen: 1.08 ng/ul
RT: 21.20 min Scan# 3164
Delta R.T. 0.00 min
Lab File: BM006598.D
Acq: 21 Jul 2016 21:36

Tgt Ion:	228	Resp:	71531
Ion Ratio	Lower	Upper	
228	100		
229	22.6	16.6	25.0
226	29.6	21.0	31.4

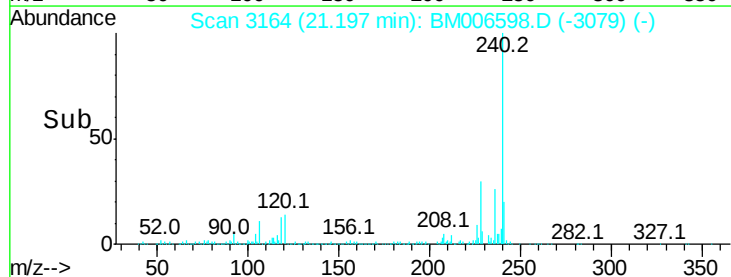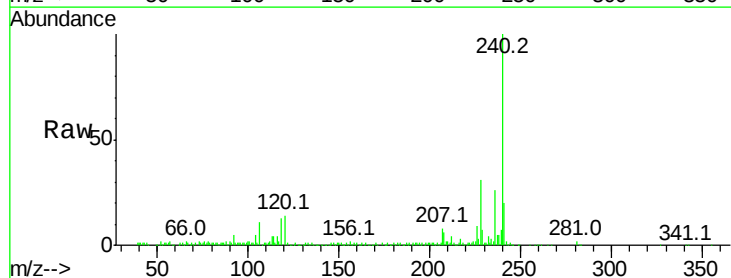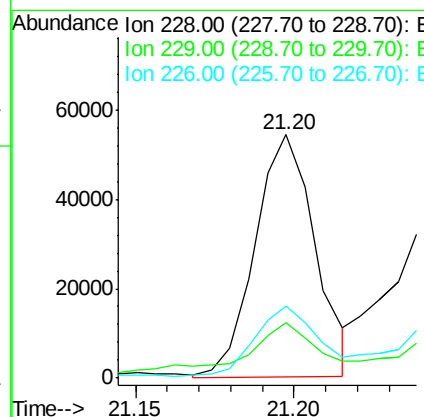

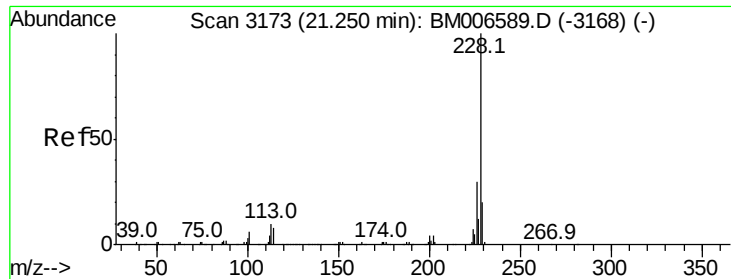





#33
Chrysene
Concen: 1.35 ng/ul
RT: 21.25 min Scan# 3173
Delta R.T. 0.00 min
Lab File: BM006589.D
Acq: 21 Jul 2016 21:36

Instrument :
BNA_M
ClientSampleId :
D9YR5

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.4	23.4	35.2
229	21.0	16.2	24.2




Manual Integrations


umangi
7/22/2016 6:24:31 PM

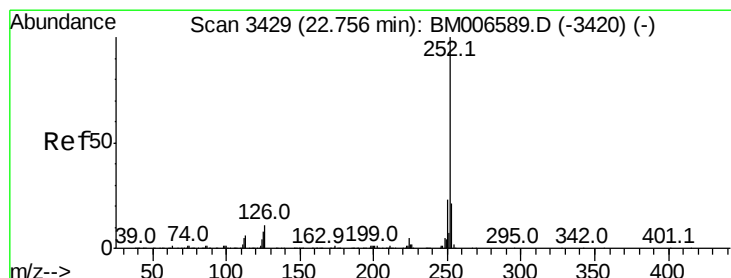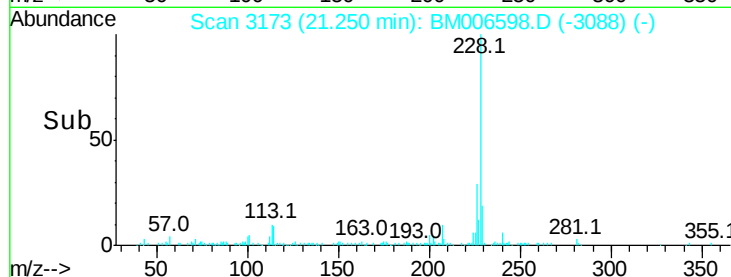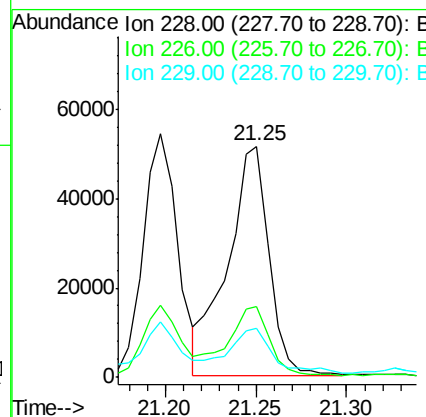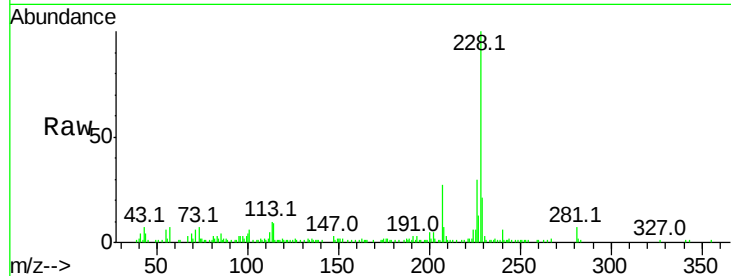

#35
Benzo(b)fluoranthene
Concen: 1.69 ng/ul
RT: 22.76 min Scan# 3429
Delta R.T. 0.00 min
Lab File: BM006589.D
Acq: 21 Jul 2016 21:36

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	18.1	27.1
125	10.5	7.6	11.4

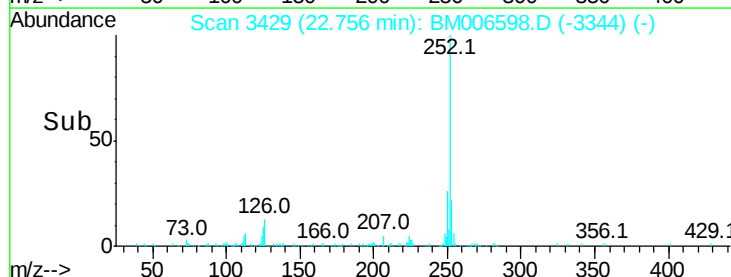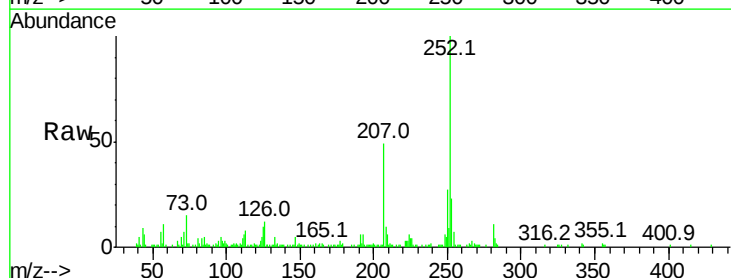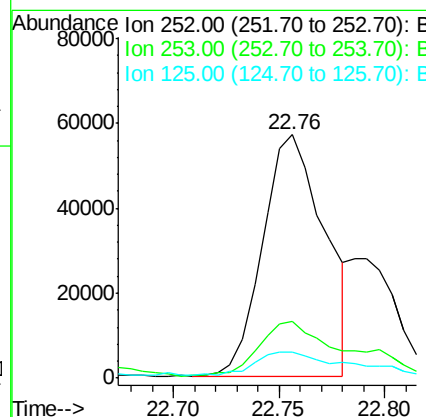

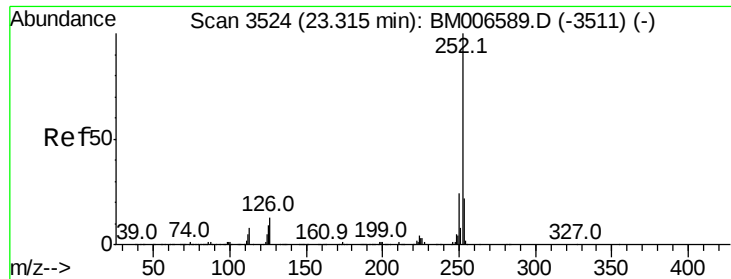

#38

Benzo(a)pyrene

Concen: 1.17 ng/ul

RT: 23.31 min Scan# 3524

Delta R.T. 0.00 min

Lab File: BM006598.D

Acq: 21 Jul 2016 21:36

Instrument :

BNA_M

ClientSampleId :

D9YR5

Tot Ion: 252 Resp: 78002

Ion Ratio Lower Upper

252 100

253 23.1 17.4 26.0

125 11.7 8.2 12.2

Manual Integrations

umangi

7/22/2016 6:24:31 PM

