
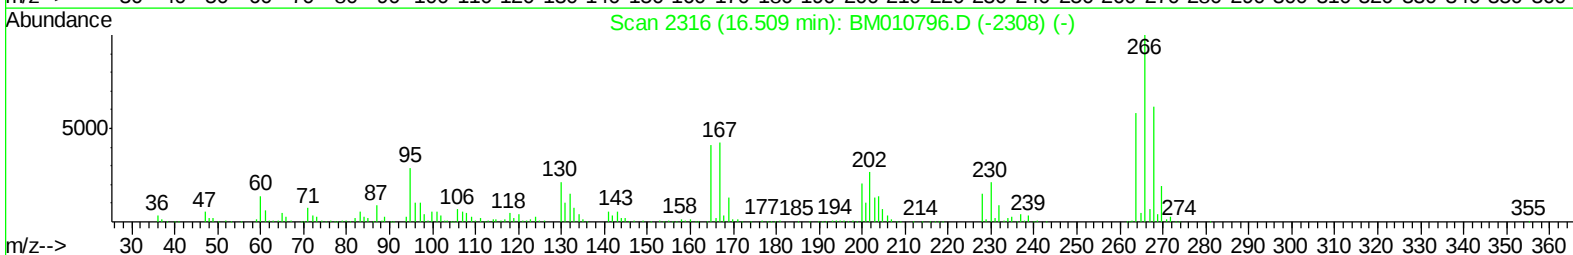
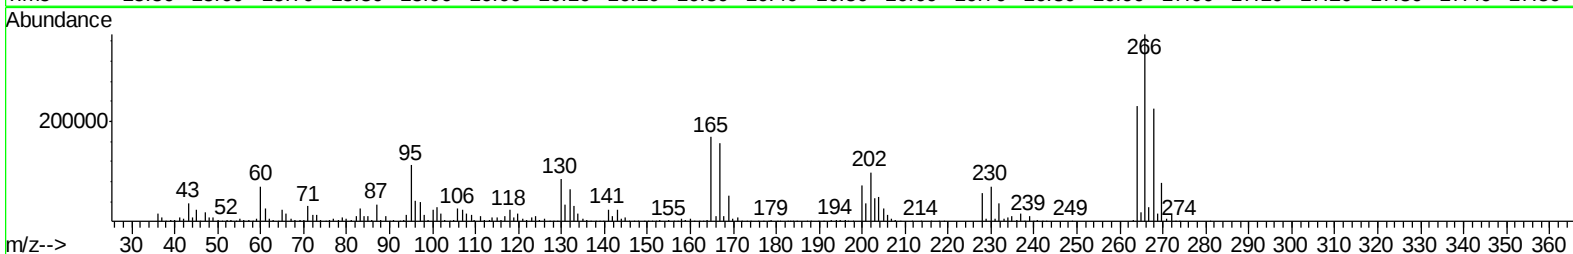


Data File : BM010937.D
Acq On : 21 Jul 2017 15:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 05:36:47 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

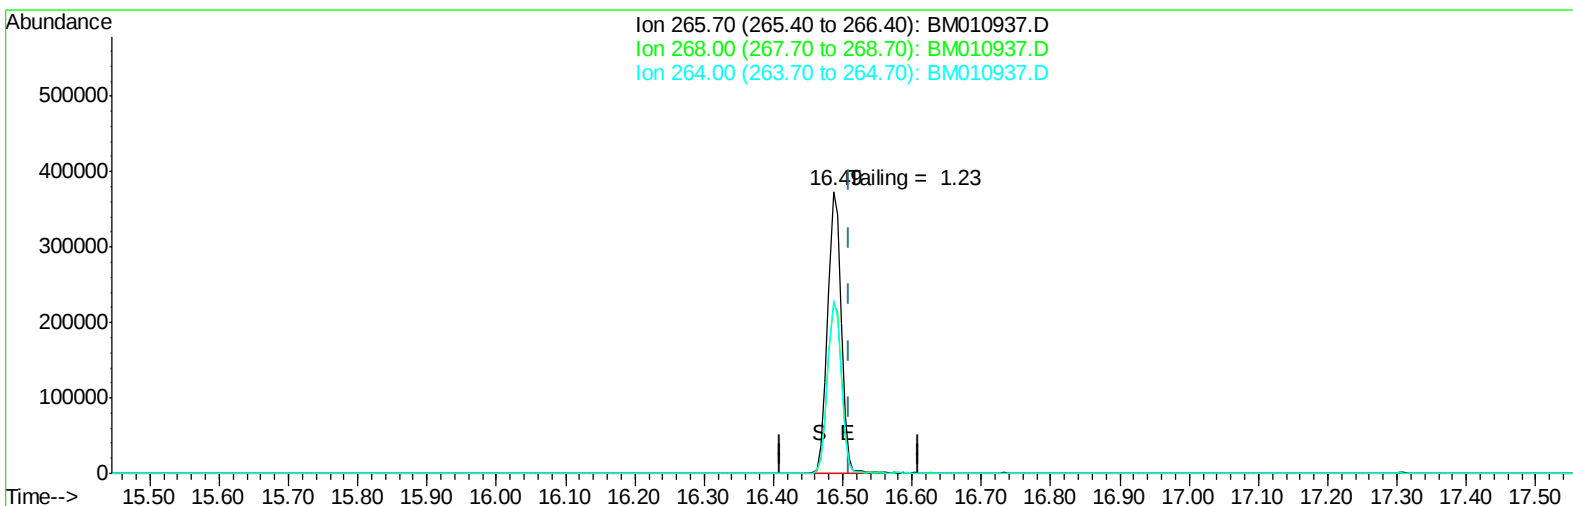

TIC: BM010937.D

(69) Pentachlorophenol (C)

16.486min (-0.023) 87913.96ng

response 508816

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.41
264.00	61.20	61.42
0.00	0.00	0.00