


Data Path : Z:\HPCHEM1\BNA M\DATA\BM072117\  
 Data File : BM010937.D  
 Acq On : 21 Jul 2017 15:58  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-BM071217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jul 12 14:21:16 2017

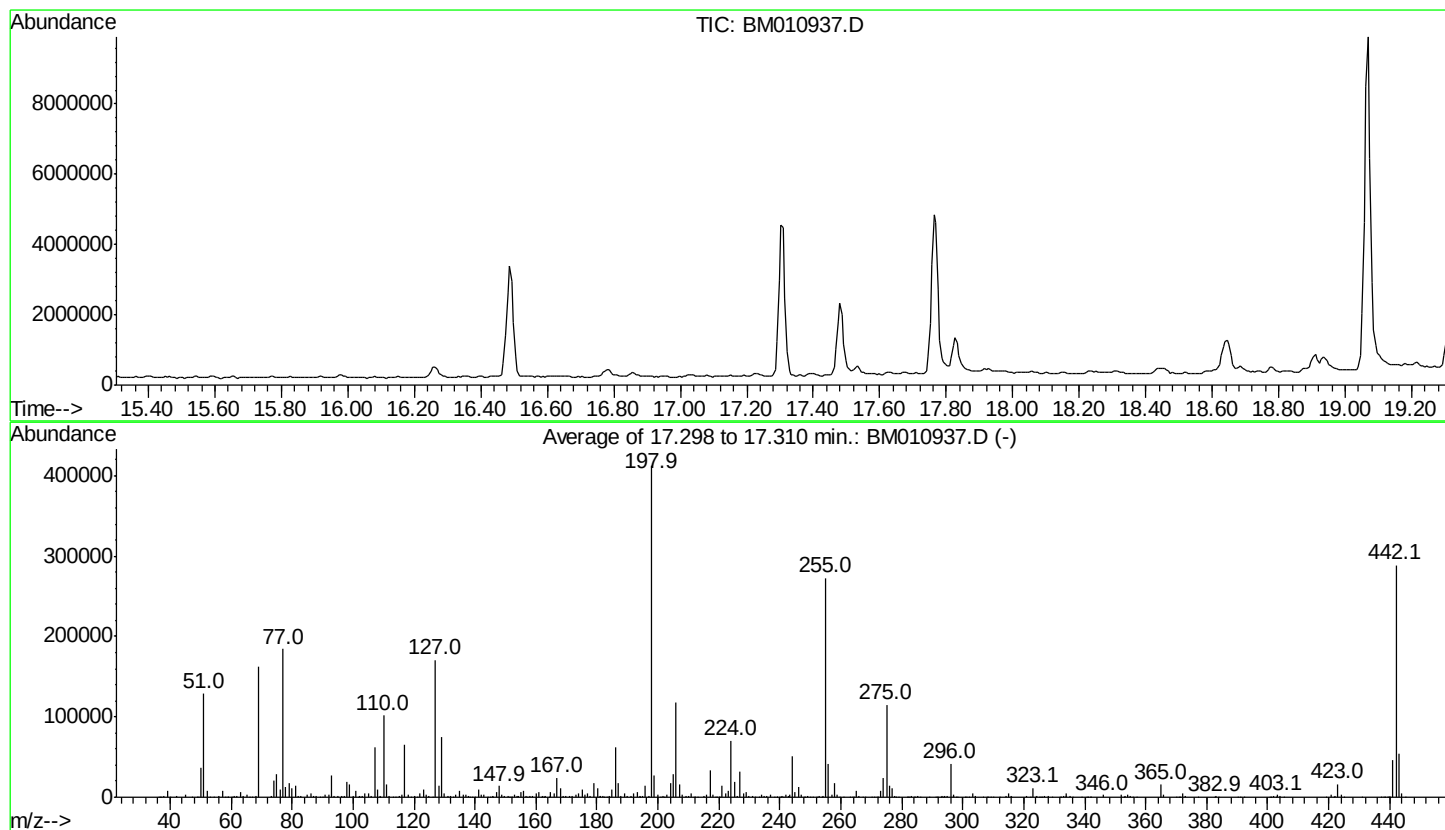

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.3      | 128940  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 2075    | PASS             |
| 69          | 198          | 0.00         | 100          | 39.3      | 162103  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 41.5      | 171069  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 2384    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 412501  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 27466   | PASS             |
| 275         | 198          | 10           | 60           | 28.0      | 115314  | PASS             |
| 365         | 198          | 1            | 100          | 3.8       | 15862   | PASS             |
| 441         | 443          | 0.01         | 100          | 84.8      | 46322   | PASS             |
| 442         | 198          | 50           | 100          | 70.0      | 288554  | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 54594   | PASS             |