

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072120\
 Data File : BM026807.D
 Acq On : 21 Jul 2020 14:36
 Operator : JU/CG
 Sample : L3336-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-1

Manual Integrations
 APPROVED

Sohil
 7/24/2020 12:03:55 PM

Quant Time: Jul 21 15:09:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 21 10:10:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.30	152	65435	20.00	ng/ul	0.00
18) Naphthalene-d8	10.05	136	274965	20.00	ng/ul	0.00
36) Acenaphthene-d10	13.97	164	171889	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.72	188	383161	20.00	ng/ul	0.00
78) Chrysene-d12	20.95	240	415035	20.00	ng/ul	0.00
86) Perylene-d12	23.02	264	421193	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.90	96	9905	4.55	ng/uL	0.00
5) Phenol-d5	6.52	99	40650	6.78	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.66	67	116439	28.73	ng/ul	0.00
9) 2-Chlorophenol-d4	6.84	132	104556	22.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.03	113	75795	15.81	ng/ul	0.00
19) Nitrobenzene-d5	8.45	128	62065	28.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.17	143	68336	29.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.70	165	118161	26.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.25	131	8475m	1.77	ng/ul	0.04
44) Dimethylphthalate-d6	13.40	166	459518	33.51	ng/ul	0.00
47) Acenaphthylene-d8	13.65	160	497891	30.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.26	143	10385	5.25	ng/ul	0.04
58) Fluorene-d10	14.97	176	388712	32.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.12	200	71152	29.72	ng/ul	0.00
71) Anthracene-d10	16.82	188	657369	34.84	ng/ul	0.00
79) Pyrene-d10	19.14	212	786137	36.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.89	264	821100	36.12	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.44	163	42430	2.956	ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072120\
Data File : BM026807.D
Acq On : 21 Jul 2020 14:36
Operator : JU/CG
Sample : L3336-03
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
PMW-1

Manual Integrations
APPROVED

Sohil
7/24/2020 12:03:55 PM

Quant Time: Jul 21 15:09:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 21 10:10:59 2020
Response via : Initial Calibration

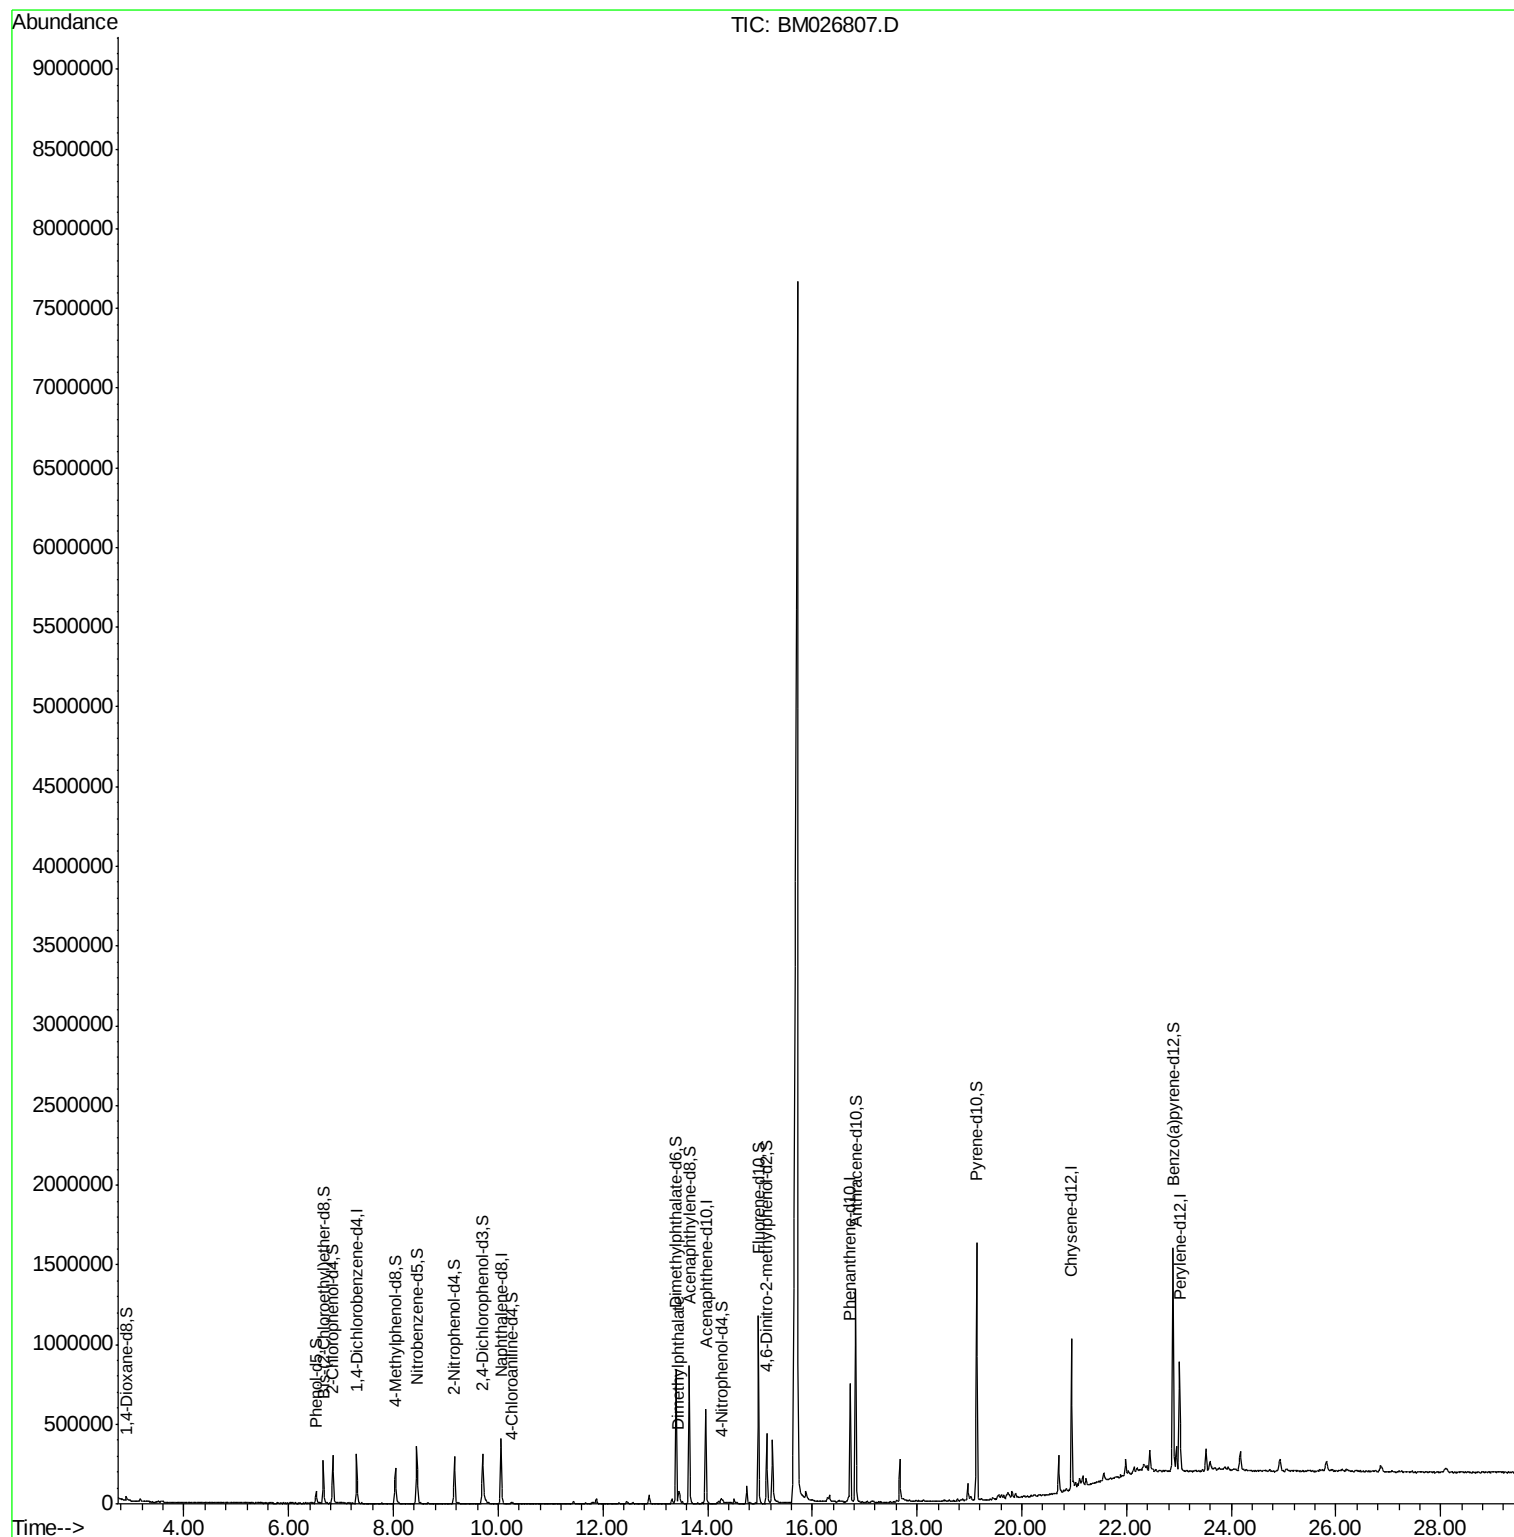

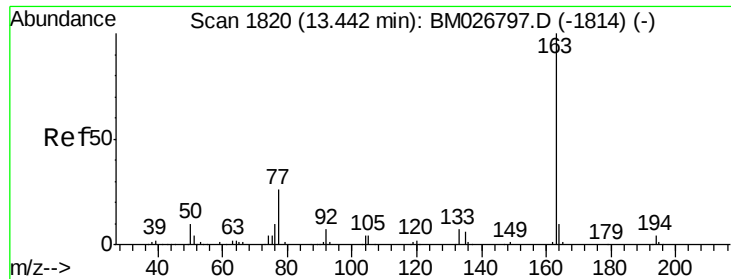

#45
 Dimethylphthalate
 Concen: 2.956 ng/ul
 RT: 13.44 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BM026807.D
 Acq: 21 Jul 2020 14:36

Instrument :
 BNA_M
 ClientSampleId :
 PMW-1

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.5	5.3
164	10.9	7.8	11.6

Manual Integrations
 APPROVED

Sohil
 7/24/2020 12:03:55 PM

