

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072120\
 Data File : BM026815.D
 Acq On : 21 Jul 2020 19:30
 Operator : JU/CG
 Sample : L3336-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 PMW-6

Manual Integrations
 APPROVED

Sohil
 7/24/2020 12:03:59 PM

Quant Time: Jul 22 01:54:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 21 10:10:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.30	152	82273	20.00	ng/ul	0.00
18) Naphthalene-d8	10.05	136	337943	20.00	ng/ul	0.00
36) Acenaphthene-d10	13.97	164	210999	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.72	188	446097	20.00	ng/ul	0.00
78) Chrysene-d12	20.95	240	463391	20.00	ng/ul	0.00
86) Perylene-d12	23.01	264	477493	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.90	96	14801	5.41	ng/uL	0.00
5) Phenol-d5	6.52	99	91820	12.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.66	67	169652	33.29	ng/ul	0.00
9) 2-Chlorophenol-d4	6.84	132	162900	28.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.03	113	132727	22.02	ng/ul	0.00
19) Nitrobenzene-d5	8.45	128	96703	36.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.16	143	110717	38.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.70	165	198167	35.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.22	131	52196m	8.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.39	166	712794	42.35	ng/ul	0.00
47) Acenaphthylene-d8	13.65	160	796058	39.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.24	143	23712m	9.76	ng/ul	0.02
58) Fluorene-d10	14.97	176	592155	40.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.12	200	107754	38.66	ng/ul	0.00
71) Anthracene-d10	16.82	188	929573	42.31	ng/ul	0.00
79) Pyrene-d10	19.14	212	1067346	44.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.89	264	1154707	44.81	ng/ul	0.00

Target Compounds				Ovalue	
45) Dimethylphthalate	13.44	163	59070	3.353	ng/ul# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072120\
Data File : BM026815.D
Acq On : 21 Jul 2020 19:30
Operator : JU/CG
Sample : L3336-08
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
PMW-6

Quant Time: Jul 22 01:54:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 21 10:10:59 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
7/24/2020 12:03:59 PM

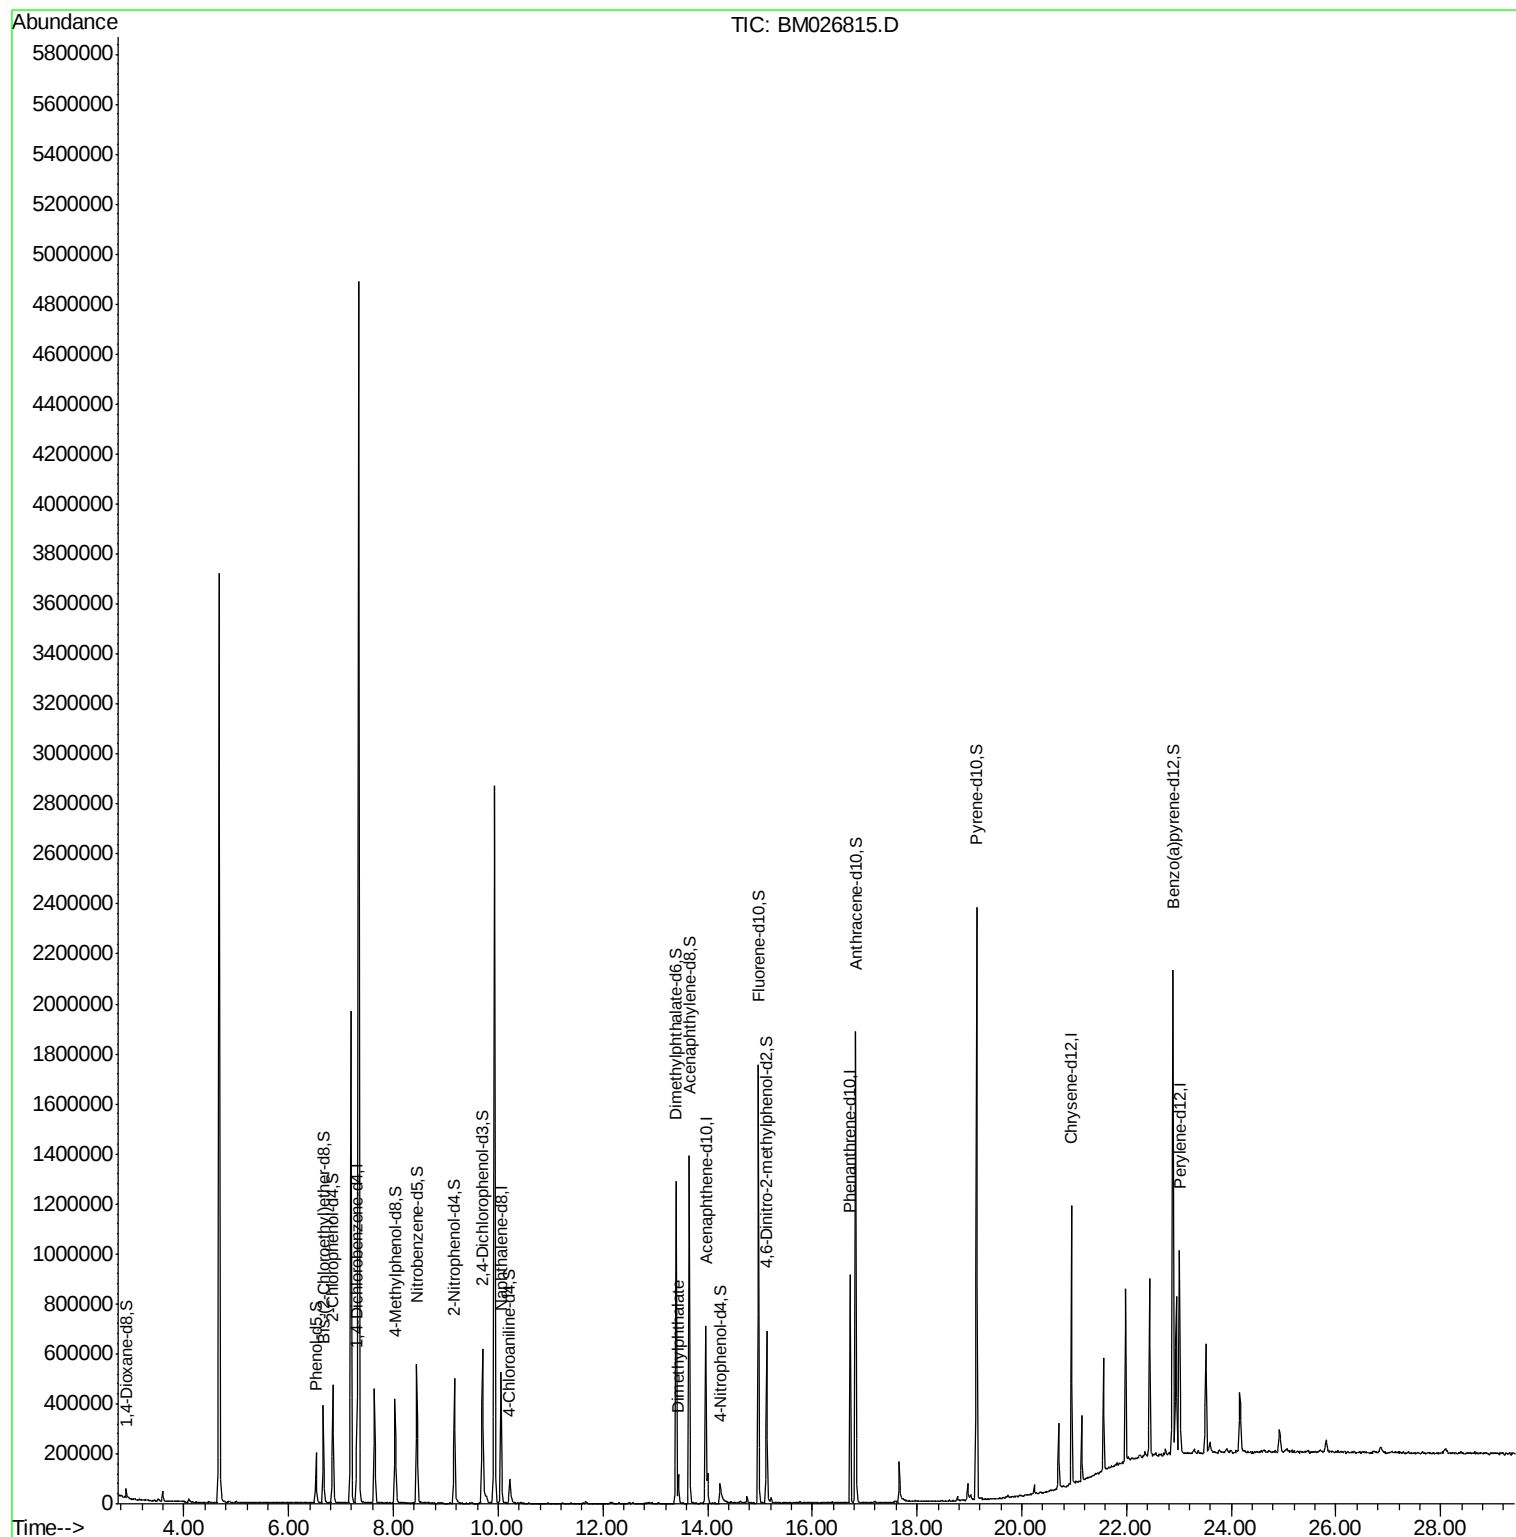

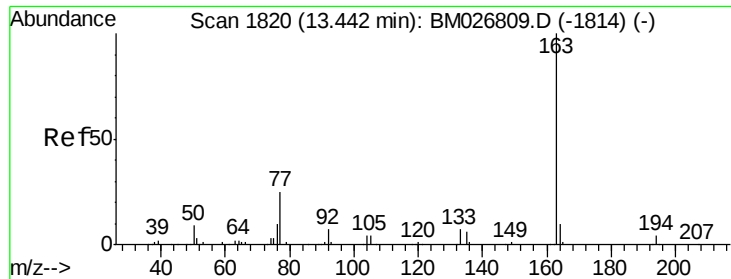

#45
 Dimethylphthalate
 Concen: 3.353 ng/ul
 RT: 13.44 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BM026815.D
 Acq: 21 Jul 2020 19:30

Instrument :
 BNA_M
 ClientSampleId :
 PMW-6

Tot Ion	Ratio	Resp	Lower	Upper
163	100	59070		
194	4.7		3.5	5.3
164	12.0		7.8	11.6

Manual Integrations
 APPROVED

Sohil
 7/24/2020 12:03:59 PM

