

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
 Data File : BM031042.D
 Acq On : 21 Jul 2021 13:13
 Operator : CG/JU
 Sample : PB137690BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB137690BL

Quant Time: Jul 21 13:58:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 21 11:41:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	69572	20.000	ng	0.00
21) Naphthalene-d8	10.404	136	292182	20.000	ng	0.00
39) Acenaphthene-d10	14.263	164	204363	20.000	ng	-0.01
64) Phenanthrene-d10	17.015	188	470028	20.000	ng	0.00
76) Chrysene-d12	21.198	240	528413	20.000	ng	-0.01
86) Perylene-d12	23.380	264	549187	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.257	112	621283	160.357	ng	0.00
7) Phenol-d6	6.822	99	804398	143.223	ng	0.00
23) Nitrobenzene-d5	8.787	82	522891	89.855	ng	0.00
42) 2,4,6-Tribromophenol	15.763	330	346275	129.758	ng	0.00
45) 2-Fluorobiphenyl	12.886	172	1211648	88.463	ng	0.00
79) Terphenyl-d14	19.656	244	2595987	97.202	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
Data File : BM031042.D
Acq On : 21 Jul 2021 13:13
Operator : CG/JU
Sample : PB137690BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137690BL

Quant Time: Jul 21 13:58:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 11:41:39 2021
Response via : Initial Calibration




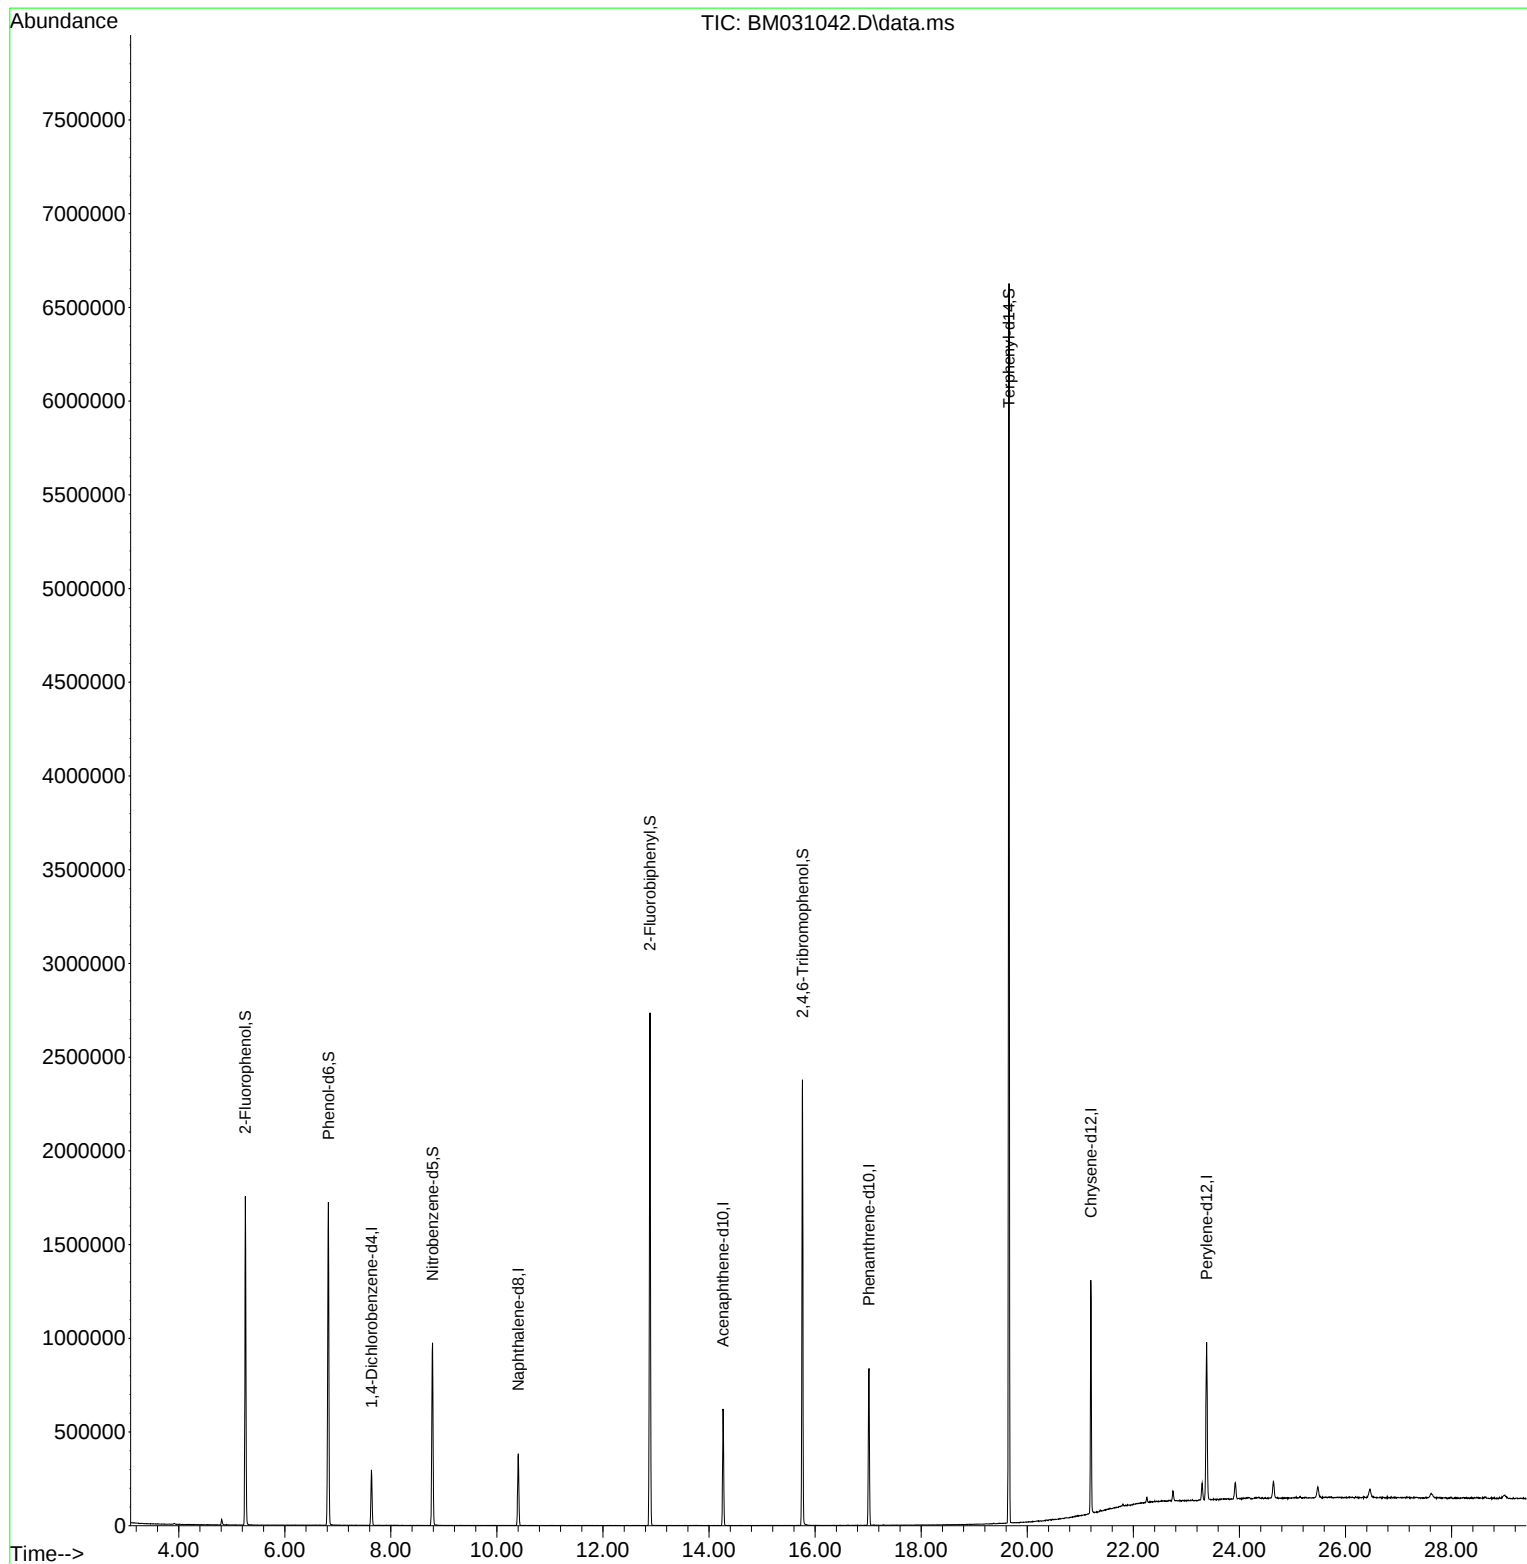


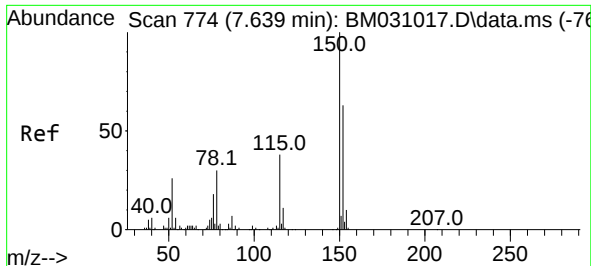

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.634 min Scan# 773
Delta R.T. -0.005 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13




Instrument :
BNA_M
ClientSampleId :
PB137690BL


Tgt Ion:152 Resp: 69572
Ion Ratio Lower Upper
152 100
150 155.9 125.9 188.9
115 60.3 44.6 67.0

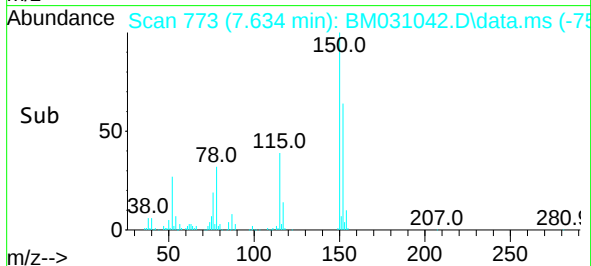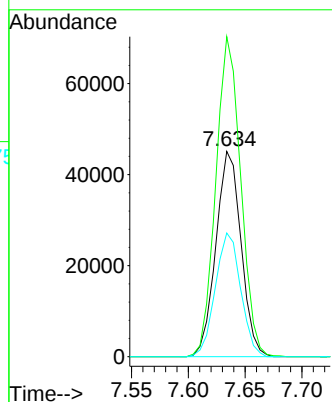

#5
2-Fluorophenol
Concen: 160.357 ng
RT: 5.257 min Scan# 369
Delta R.T. 0.000 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Tgt Ion:112 Resp: 621283
Ion Ratio Lower Upper
112 100
64 60.7 47.1 70.7
63 37.5 27.3 40.9


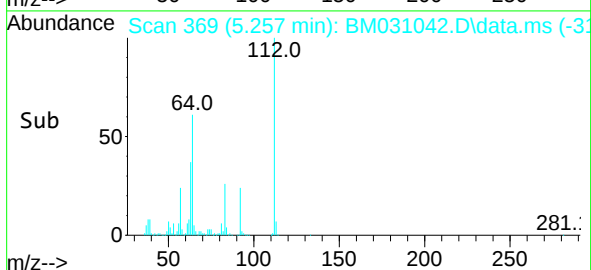
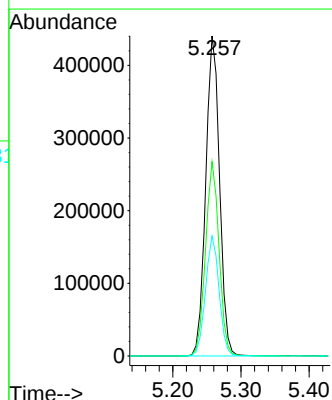
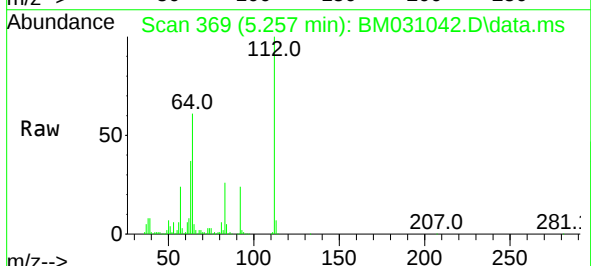


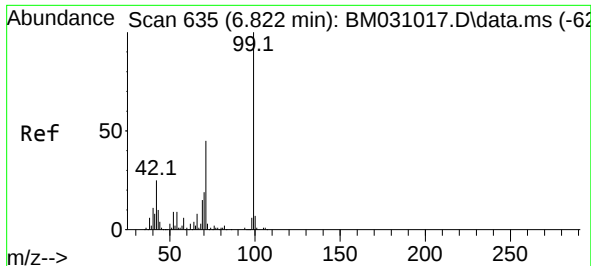

#7
Phenol-d6
Concen: 143.223 ng
RT: 6.822 min Scan# 635
Delta R.T. 0.000 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13




Instrument :
BNA_M
ClientSampleId :
PB137690BL


Tgt Ion: 99 Resp: 804398
Ion Ratio Lower Upper
99 100
42 24.1 18.0 27.0
71 43.9 30.9 46.3

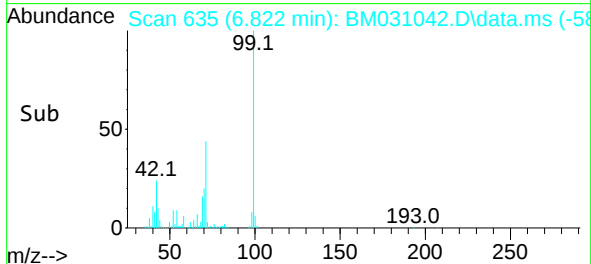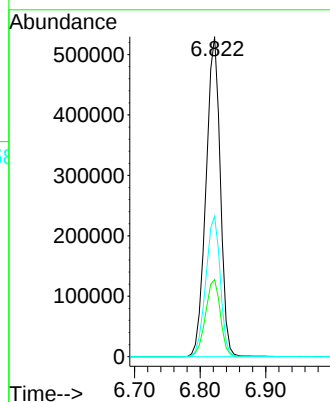

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.404 min Scan# 1244
Delta R.T. -0.006 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Tgt Ion: 136 Resp: 292182
Ion Ratio Lower Upper
136 100
137 11.0 8.4 12.6
54 7.9 5.5 8.3
68 4.3 4.2 6.2


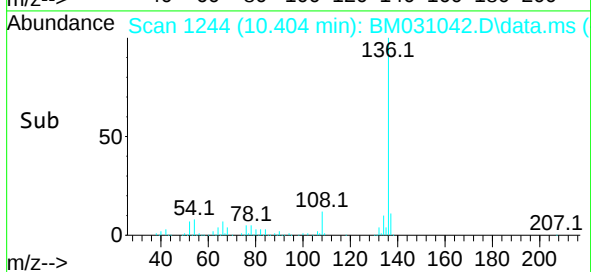
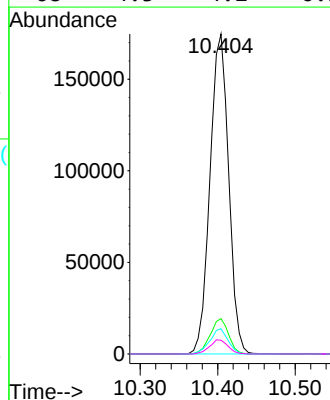
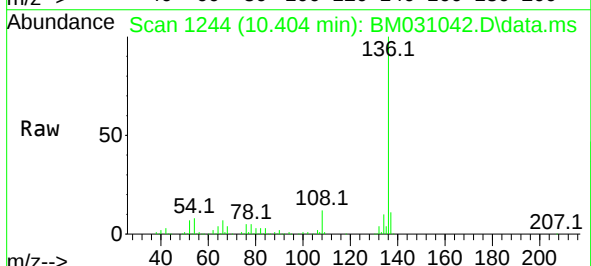


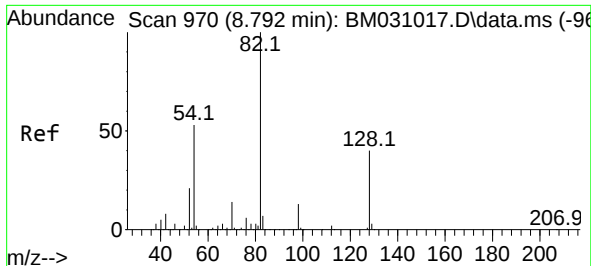

#23
Nitrobenzene-d5
Concen: 89.855 ng
RT: 8.787 min Scan# 969
Delta R.T. -0.006 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13




Instrument :
BNA_M
ClientSampleId :
PB137690BL


Tgt Ion: 82 Resp: 522891
Ion Ratio Lower Upper
82 100
128 39.1 31.1 46.7
54 53.0 37.3 55.9

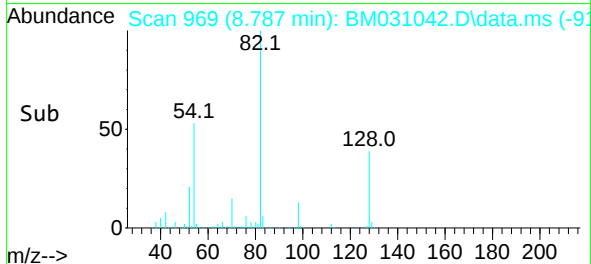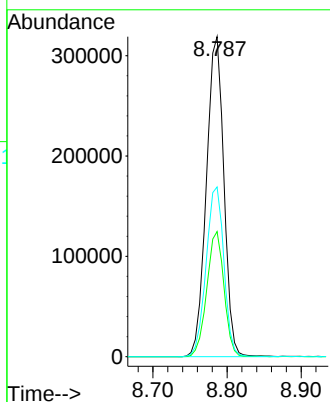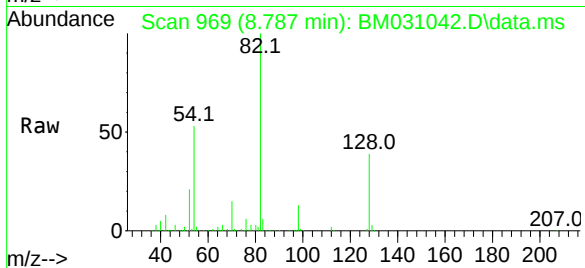

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.263 min Scan# 1900
Delta R.T. -0.012 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Tgt Ion: 164 Resp: 204363
Ion Ratio Lower Upper
164 100
162 98.7 83.4 125.0
160 44.4 37.2 55.8


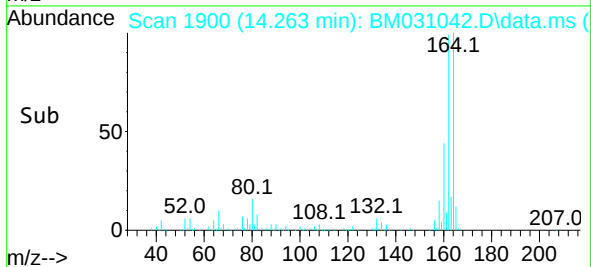
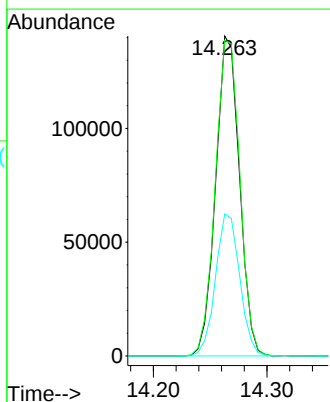
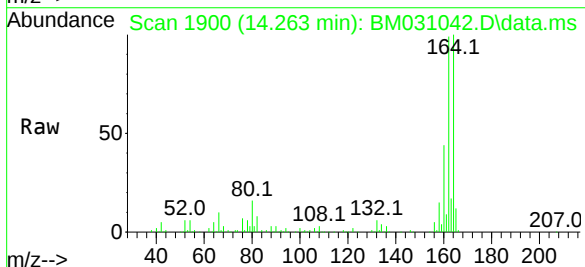


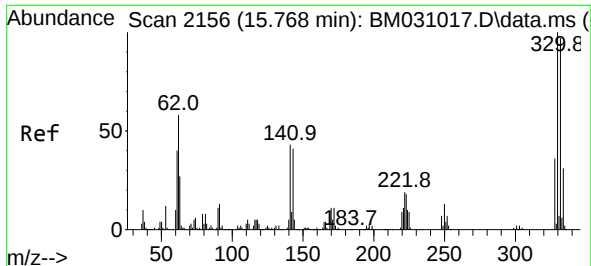

#42
2,4,6-Tribromophenol
Concen: 129.758 ng
RT: 15.763 min Scan# 2155
Delta R.T. -0.006 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13




Instrument :
BNA_M
ClientSampleId :
PB137690BL


Tgt Ion:330 Resp: 346275
Ion Ratio Lower Upper
330 100
332 97.2 77.0 115.4
141 48.6 30.2 45.2#

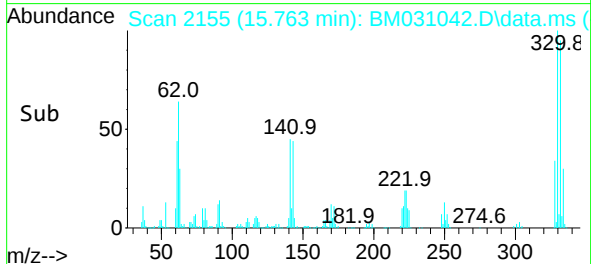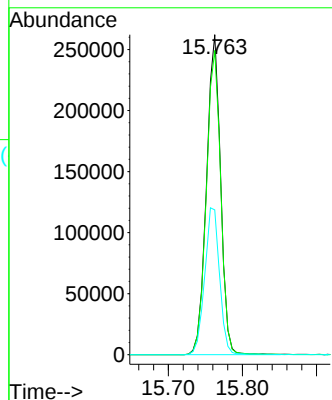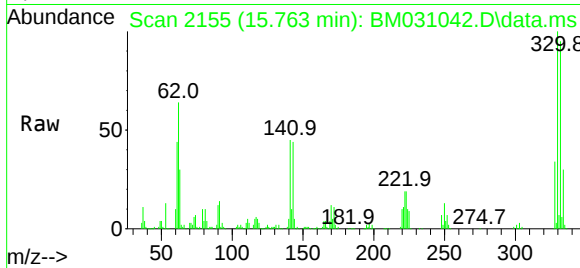

#45
2-Fluorobiphenyl
Concen: 88.463 ng
RT: 12.886 min Scan# 1666
Delta R.T. -0.006 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Tgt Ion:172 Resp: 1211648
Ion Ratio Lower Upper
172 100
171 35.4 28.6 43.0
170 23.3 18.4 27.6


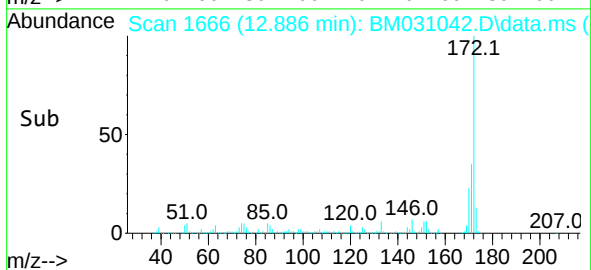
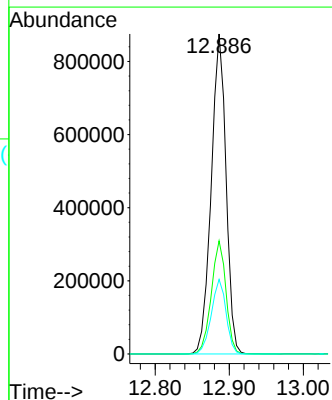
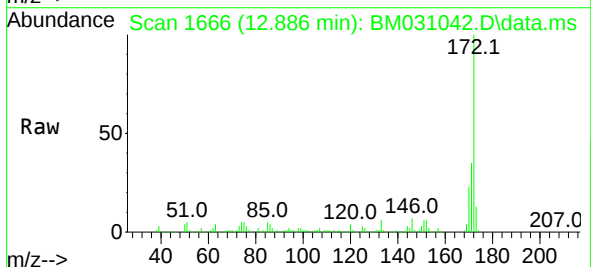




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.015 min Scan# 2368
Delta R.T. -0.006 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13




Instrument :
BNA_M
ClientSampleId :
PB137690BL


Tgt Ion:188 Resp: 470028
Ion Ratio Lower Upper
188 100
94 6.5 6.0 9.0
80 7.5 6.6 9.8

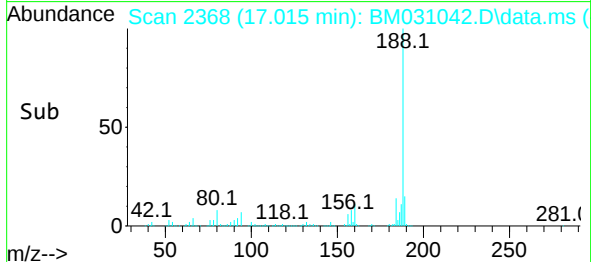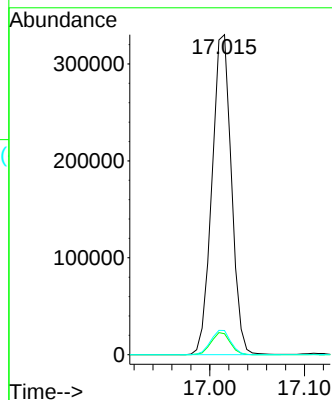

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.198 min Scan# 3079
Delta R.T. -0.012 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Tgt Ion:240 Resp: 528413
Ion Ratio Lower Upper
240 100
120 8.6 7.0 10.6
236 25.6 21.0 31.4


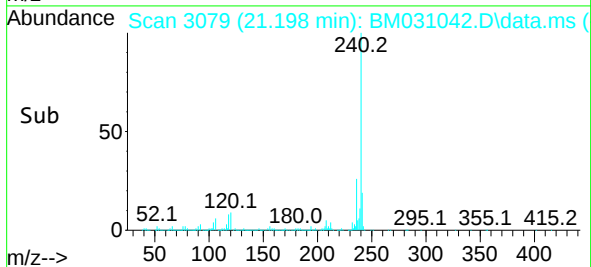
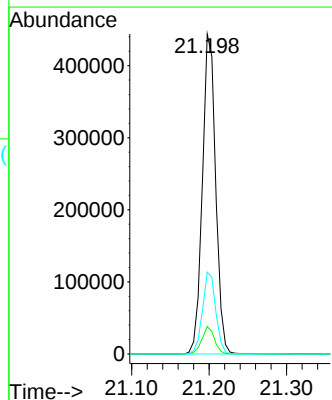
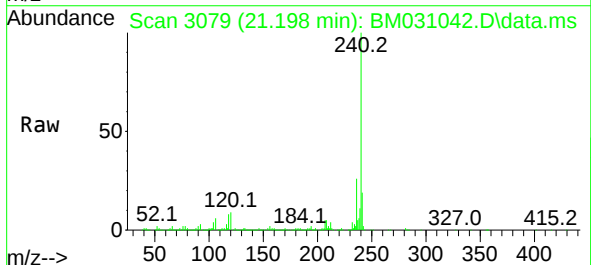


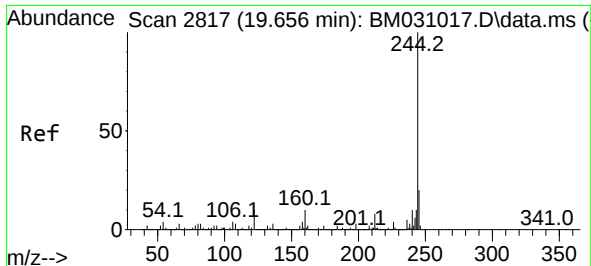

#79
Terphenyl-d14
Concen: 97.202 ng
RT: 19.656 min Scan# 2817
Delta R.T. 0.000 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Instrument :
BNA_M
ClientSampleId :
PB137690BL

Tgt Ion:244 Resp: 2595987
Ion Ratio Lower Upper
244 100
212 7.7 6.3 9.5
122 9.4 6.9 10.3

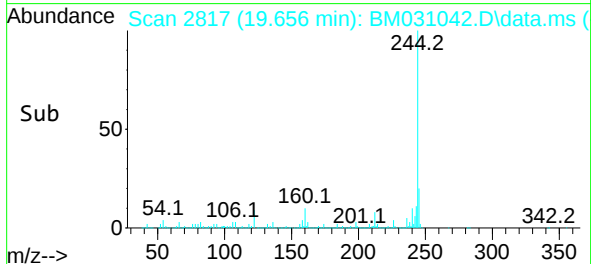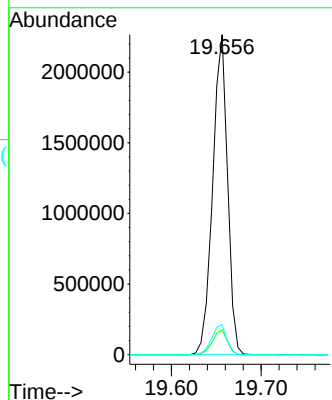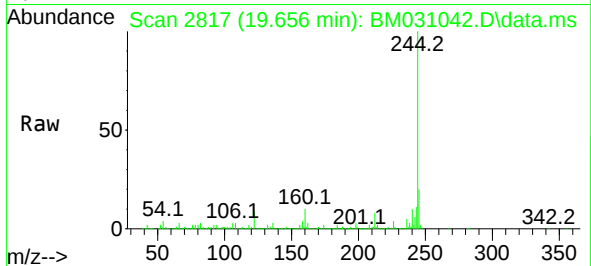

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.380 min Scan# 3450
Delta R.T. -0.012 min
Lab File: BM031042.D
Acq: 21 Jul 2021 13:13

Tgt Ion:264 Resp: 549187
Ion Ratio Lower Upper
264 100
260 22.3 19.8 29.8
265 21.4 17.7 26.5

