

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
 Data File : BM031038.D
 Acq On : 21 Jul 2021 10:27
 Operator : CG/JU
 Sample : PB137674BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB137674BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	362	369	381	rBV	1552373	2175600	31.62%	8.630%
2	6.822	627	635	647	rBV	1493433	2358794	34.29%	9.357%
3	7.634	767	773	780	rBV	253096	394637	5.74%	1.565%
4	8.786	961	969	979	rBV	846251	1420170	20.64%	5.634%
5	10.404	1236	1244	1254	rBV	338852	571598	8.31%	2.267%
6	12.886	1659	1666	1678	rBV	2274920	3353596	48.74%	13.303%
7	14.263	1894	1900	1910	rVB	552880	816471	11.87%	3.239%
8	15.757	2148	2154	2175	rBV	2163014	2962500	43.06%	11.752%
9	17.009	2361	2367	2379	rBV	758125	1079778	15.69%	4.283%
10	19.650	2810	2816	2822	rBV	5588545	6879941	100.00%	27.292%
11	21.203	3074	3080	3085	rBV	1052504	1351652	19.65%	5.362%
12	23.297	3432	3436	3442	rVB2	73655	117094	1.70%	0.464%
13	23.380	3443	3450	3459	rBV2	823738	1464624	21.29%	5.810%
14	23.921	3538	3542	3549	rVB	69677	123168	1.79%	0.489%
15	24.644	3661	3665	3673	rVB3	71379	138994	2.02%	0.551%




Sum of corrected areas: 25208617

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
Data File : BM031038.D
Acq On : 21 Jul 2021 10:27
Operator : CG/JU
Sample : PB137674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137674BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

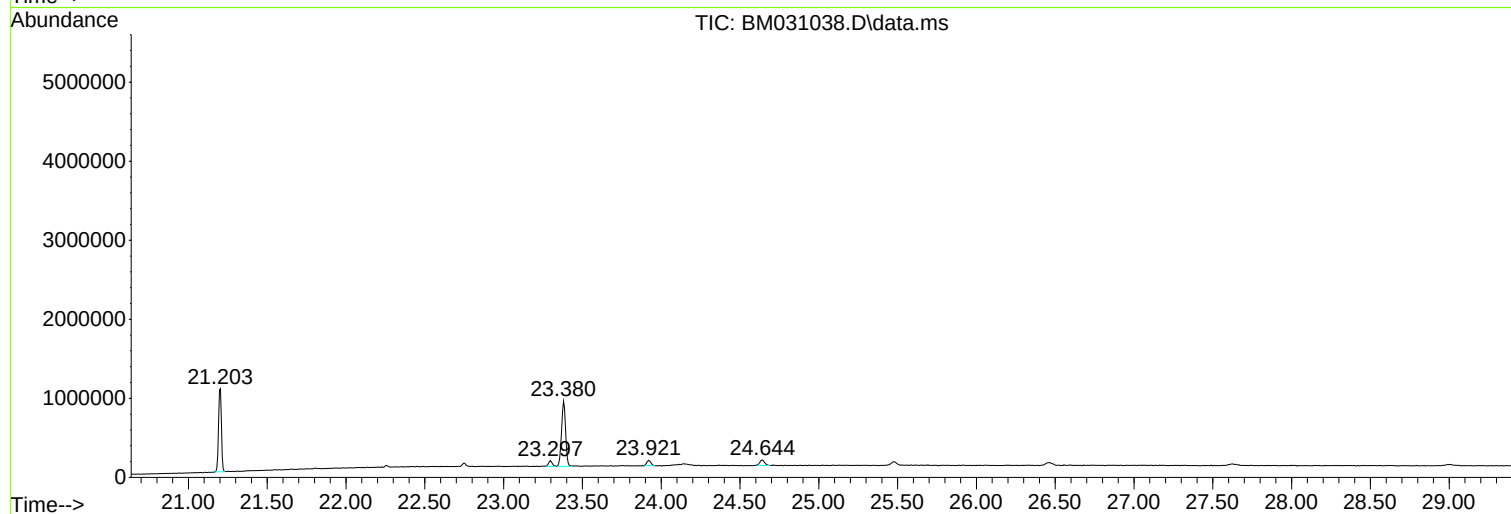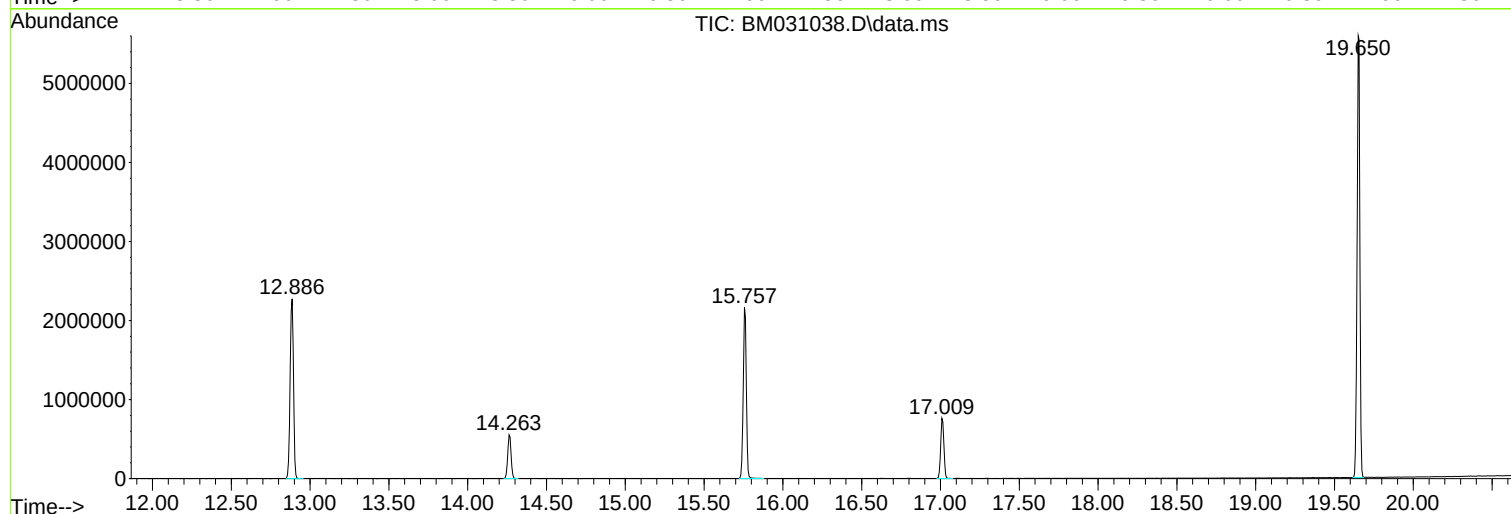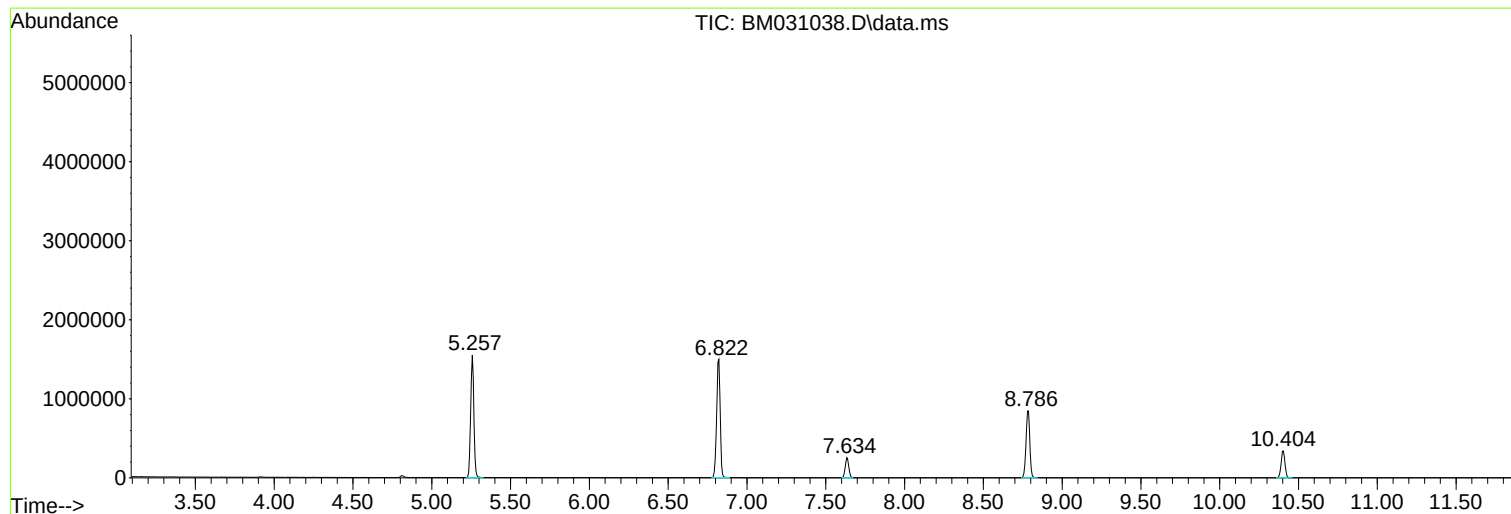

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
Data File : BM031038.D
Acq On : 21 Jul 2021 10:27
Operator : CG/JU
Sample : PB137674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137674BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
Data File : BM031038.D
Acq On : 21 Jul 2021 10:27
Operator : CG/JU
Sample : PB137674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137674BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------