
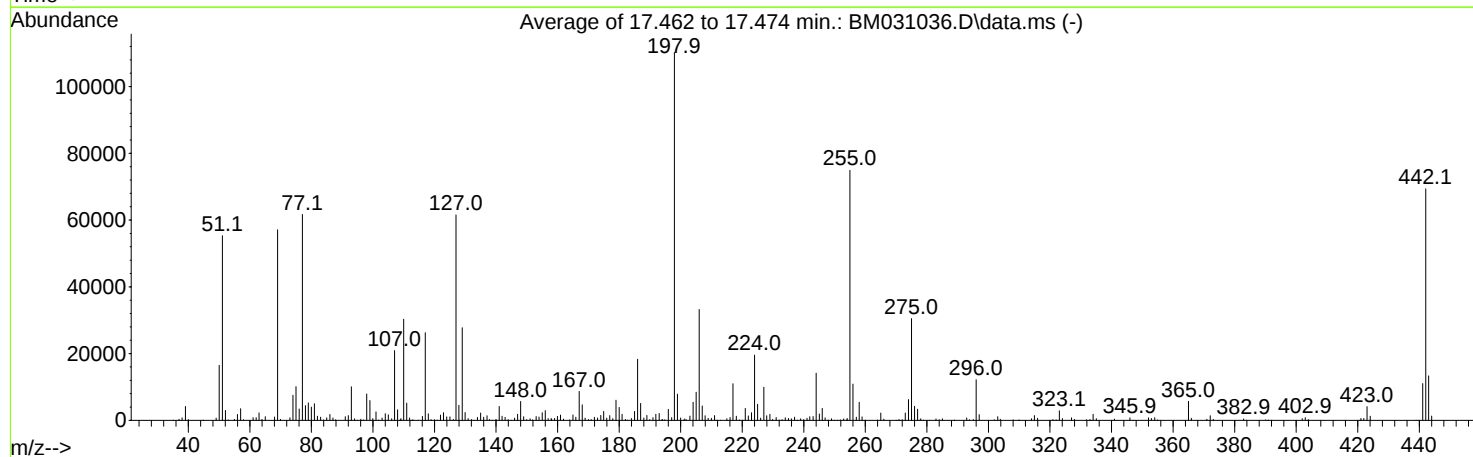


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
 Data File : BM031036.D
 Acq On : 21 Jul 2021 09:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 20 13:21:40 2021

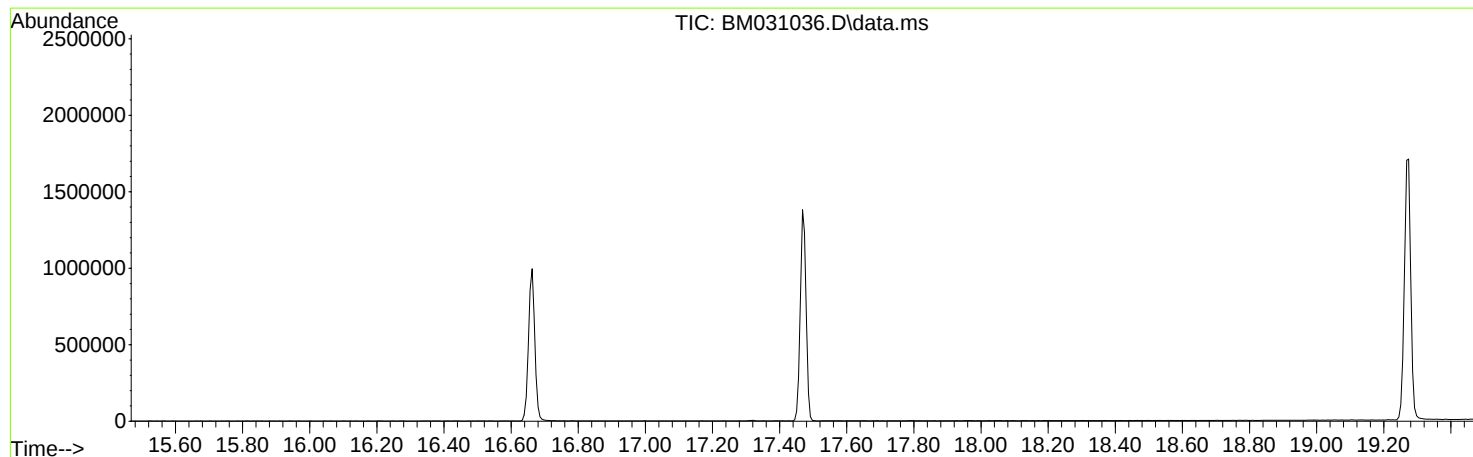

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	55299	PASS
68	69	0.00	2	1.8	1023	PASS
69	198	0.00	100	51.8	57080	PASS
70	69	0.00	2	0.5	286	PASS
127	198	10	80	55.9	61568	PASS
197	198	0.00	2	0.8	828	PASS
198	198	100	100	100.0	110203	PASS
199	198	5	9	7.1	7840	PASS
275	198	10	60	27.6	30469	PASS
365	198	1	100	5.2	5704	PASS
441	198	0.01	100	10.0	11034	PASS
442	442	50	100	100.0	69352	PASS
443	442	15	24	19.2	13314	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
7/21/2021	BNA_M	<u>BM031036.D</u>
Compound Name	Response	Retention Time
DDT	489095	20.5
DDD	4188	20.06
DDE	651	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4839	493934	0.98

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
 Data File : BM031036.D
 Acq On : 21 Jul 2021 09:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 10:56:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 13:21:40 2021
 Response via : Initial Calibration

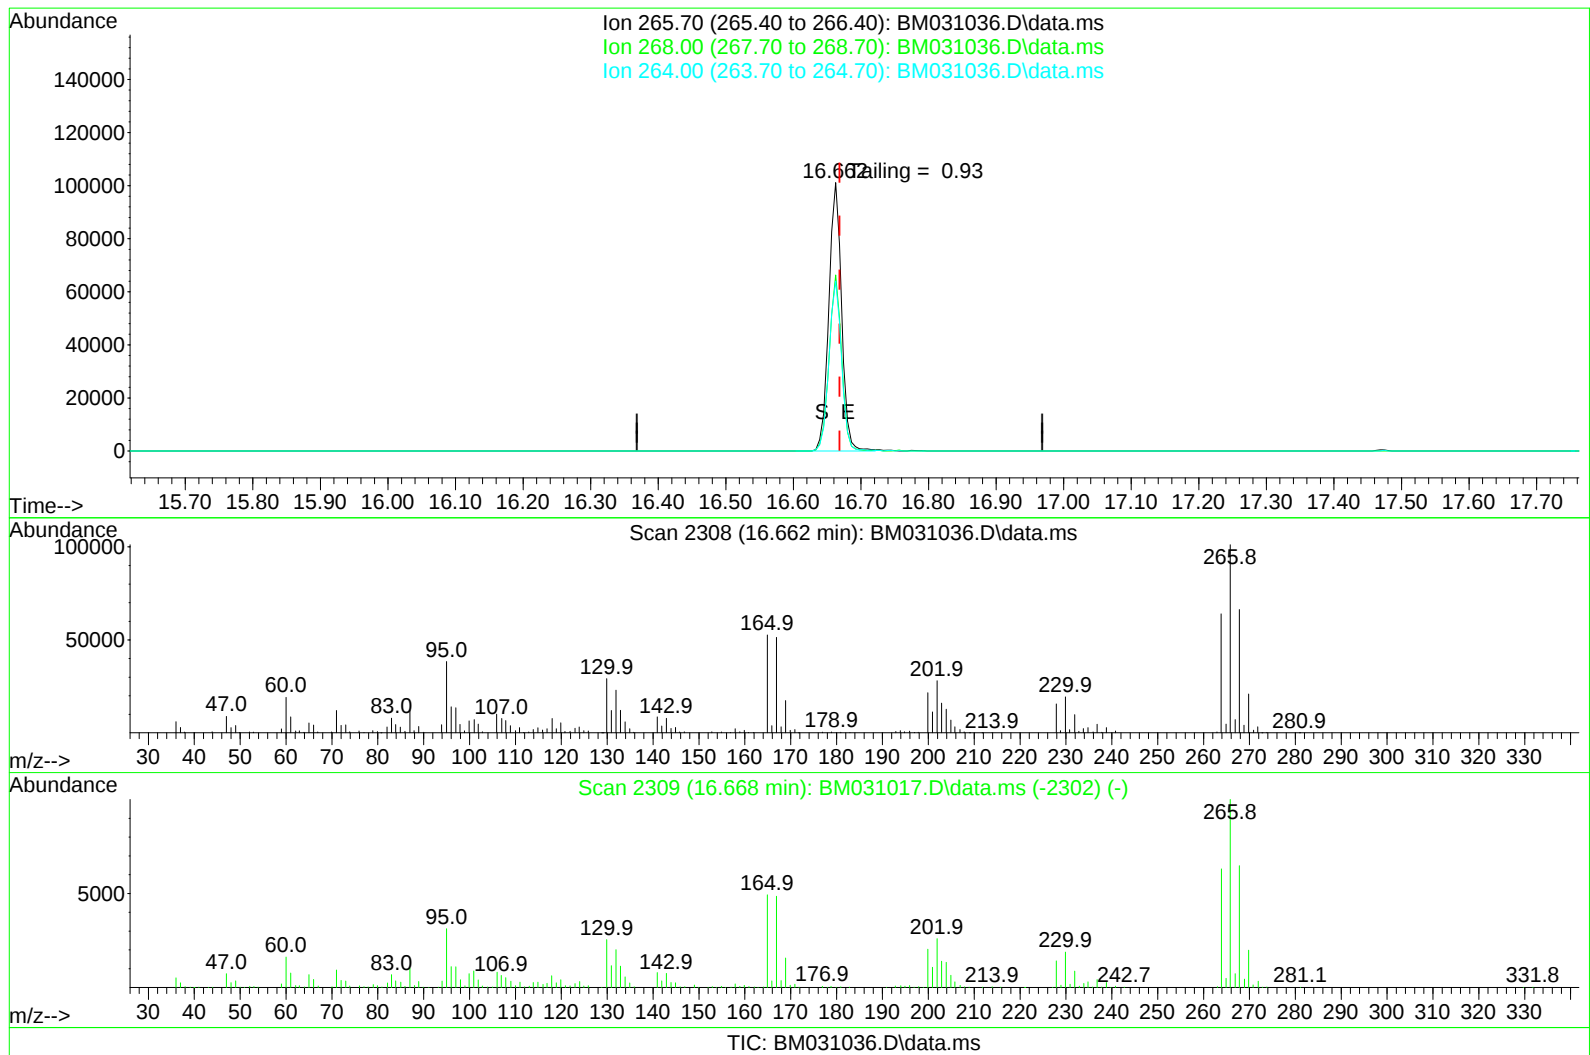

(70) Pentachlorophenol (C)

16.662min (-0.006) 0.00 ng




response 133462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.61
264.00	64.90	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072121\
Data File : BM031036.D
Acq On : 21 Jul 2021 09:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 21 10:56:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 13:21:40 2021
Response via : Initial Calibration

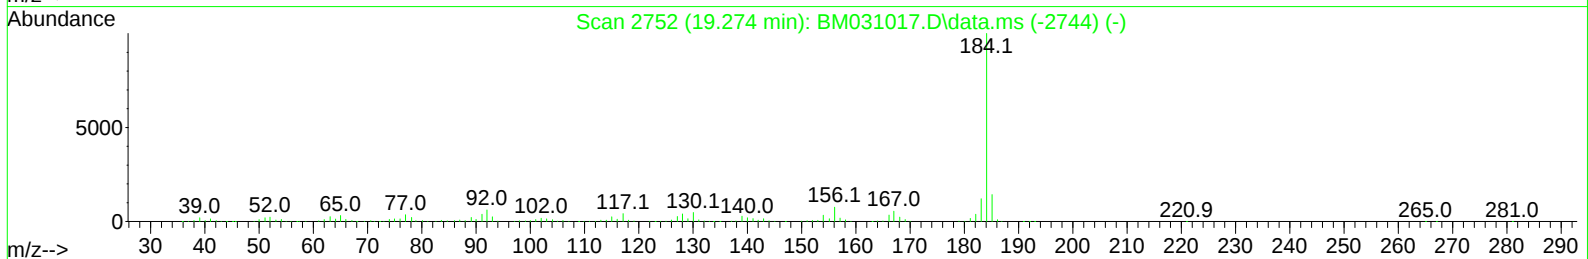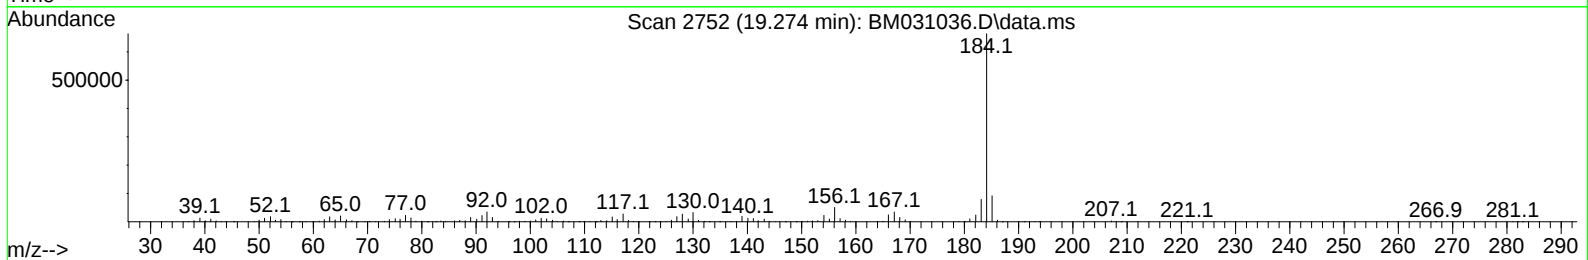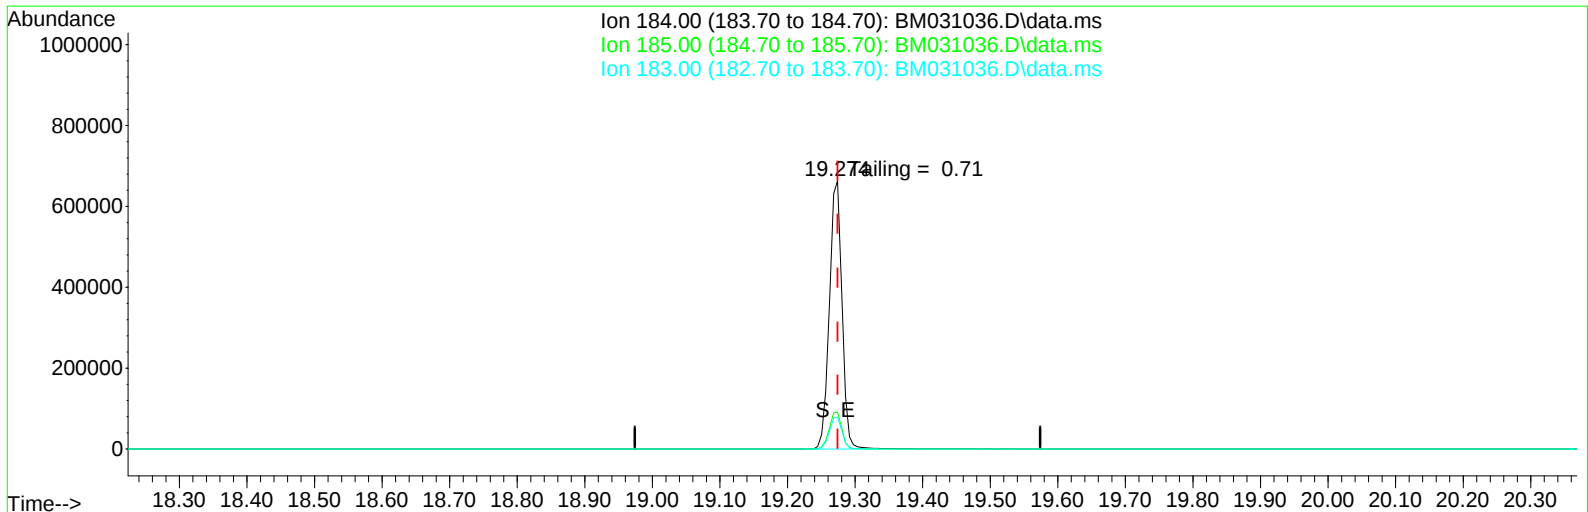

TIC: BM031036.D\data.ms

(77) Benzidine

19.274min (+ 0.000) 0.00 ng

response 864567

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.79
183.00	12.30	11.92
0.00	0.00	0.00