

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035884.D
 Acq On : 21 Jul 2022 11:31
 Operator : CG/JU
 Sample : PB146339BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146339BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	396	403	418	rBV	7869949	10898010	48.52%	10.991%
2	7.063	668	676	695	rBV	7266787	11197444	49.85%	11.292%
3	7.892	810	817	827	rBV	1225332	1927372	8.58%	1.944%
4	9.063	1007	1016	1029	rBV	4308056	6955357	30.97%	7.014%
5	10.704	1286	1295	1305	rBV	1641433	2776335	12.36%	2.800%
6	13.163	1704	1713	1727	rBV	11315505	16112439	71.74%	16.249%
7	14.527	1936	1945	1953	rBV	2466310	3556064	15.83%	3.586%
8	16.015	2189	2198	2220	rBV	8001907	11350984	50.54%	11.447%
9	17.268	2404	2411	2420	rBV	3071226	4114345	18.32%	4.149%
10	19.892	2851	2857	2872	rBV	18549509	22460626	100.00%	22.651%
11	21.445	3116	3121	3135	rBV	3310886	4115257	18.32%	4.150%
12	23.815	3517	3524	3537	rBV2	1805200	3694187	16.45%	3.726%




Sum of corrected areas: 99158420

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035884.D
Acq On : 21 Jul 2022 11:31
Operator : CG/JU
Sample : PB146339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

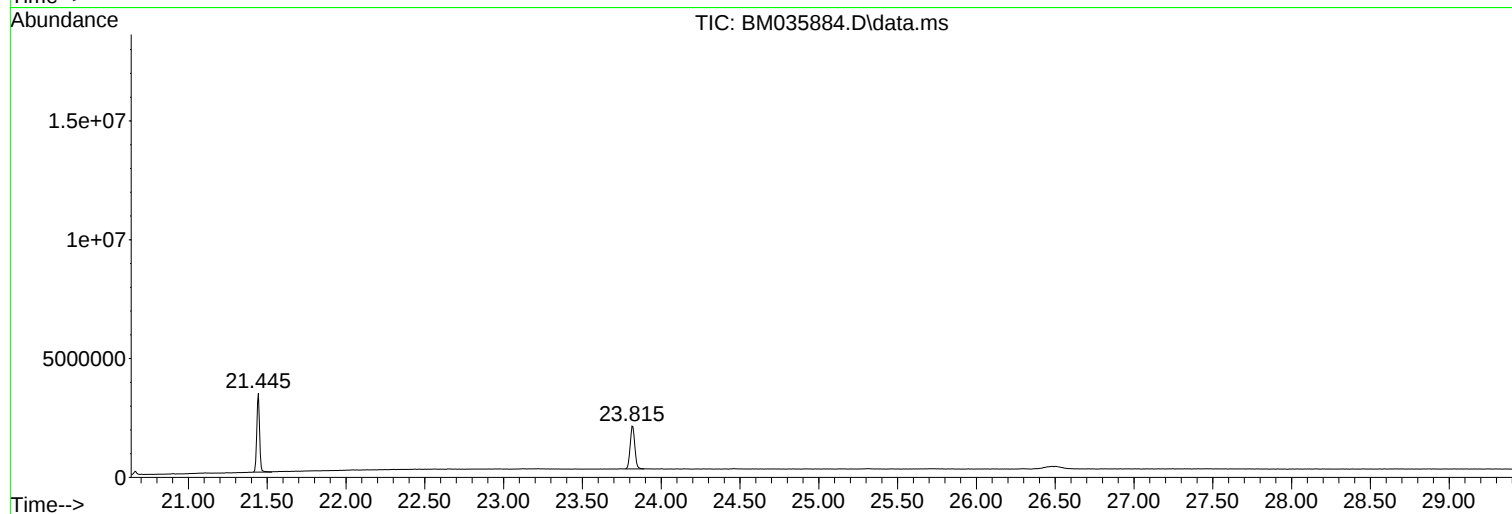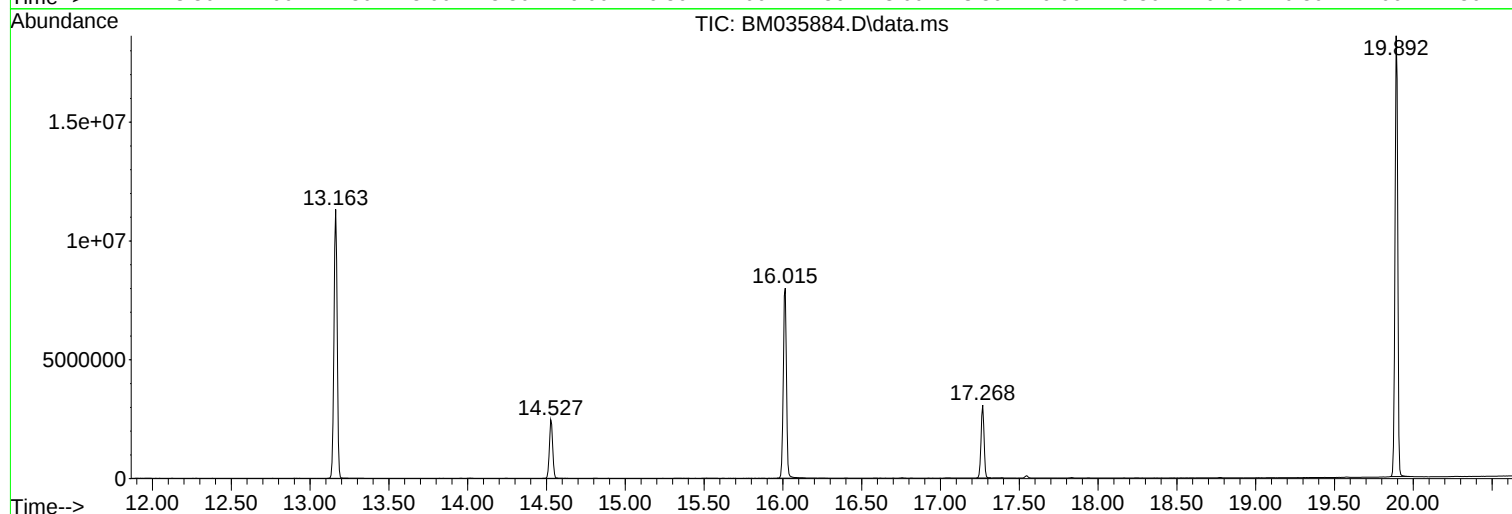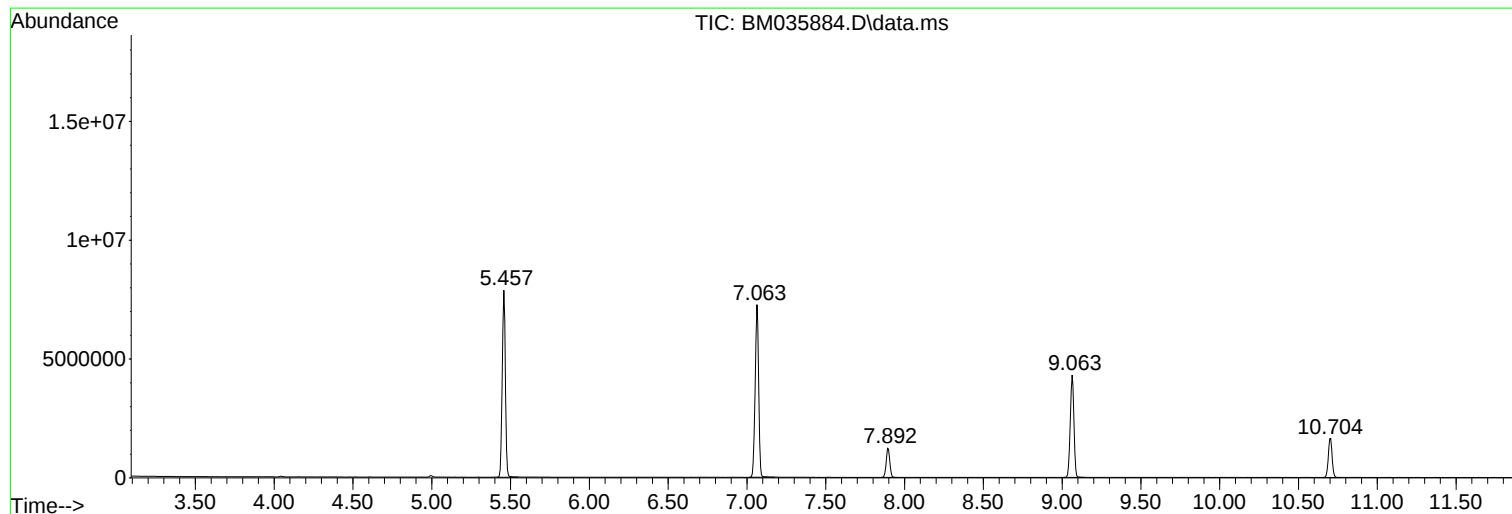

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035884.D
Acq On : 21 Jul 2022 11:31
Operator : CG/JU
Sample : PB146339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035884.D
Acq On : 21 Jul 2022 11:31
Operator : CG/JU
Sample : PB146339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------