

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035895.D
 Acq On : 21 Jul 2022 18:55
 Operator : CG/JU
 Sample : N3786-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0718-WC-TP-WC17A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.569	79	82	92	rVB	42790	64554	1.05%	0.144%
2	5.451	396	402	415	rBV	2484719	3517084	57.30%	7.828%
3	7.057	666	675	688	rBV	2463428	3755075	61.18%	8.358%
4	7.892	810	817	826	rBV	1302487	2027367	33.03%	4.512%
5	9.063	1008	1016	1027	rBV	1438962	2367444	38.57%	5.269%
6	10.698	1287	1294	1304	rBV	1727620	2904859	47.33%	6.466%
7	13.163	1705	1713	1720	rBV	3701666	5385063	87.74%	11.986%
8	14.527	1938	1945	1959	rBV	2532441	3702408	60.32%	8.241%
9	16.010	2191	2197	2213	rBV	2567521	3599514	58.65%	8.012%
10	17.268	2404	2411	2417	rBV	2922005	4004200	65.24%	8.912%
11	18.162	2559	2563	2572	rBV	75730	116090	1.89%	0.258%
12	19.892	2851	2857	2871	rBV	5096649	6137522	100.00%	13.661%
13	20.662	2985	2988	2993	rBV	121024	144276	2.35%	0.321%
14	21.168	3070	3074	3081	rBV2	119868	187541	3.06%	0.417%
15	21.444	3116	3121	3130	rBV	2895192	3620845	59.00%	8.059%
16	23.821	3518	3525	3536	rVB2	1701223	3394355	55.30%	7.555%




Sum of corrected areas: 44928197

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035895.D
Acq On : 21 Jul 2022 18:55
Operator : CG/JU
Sample : N3786-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC17A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

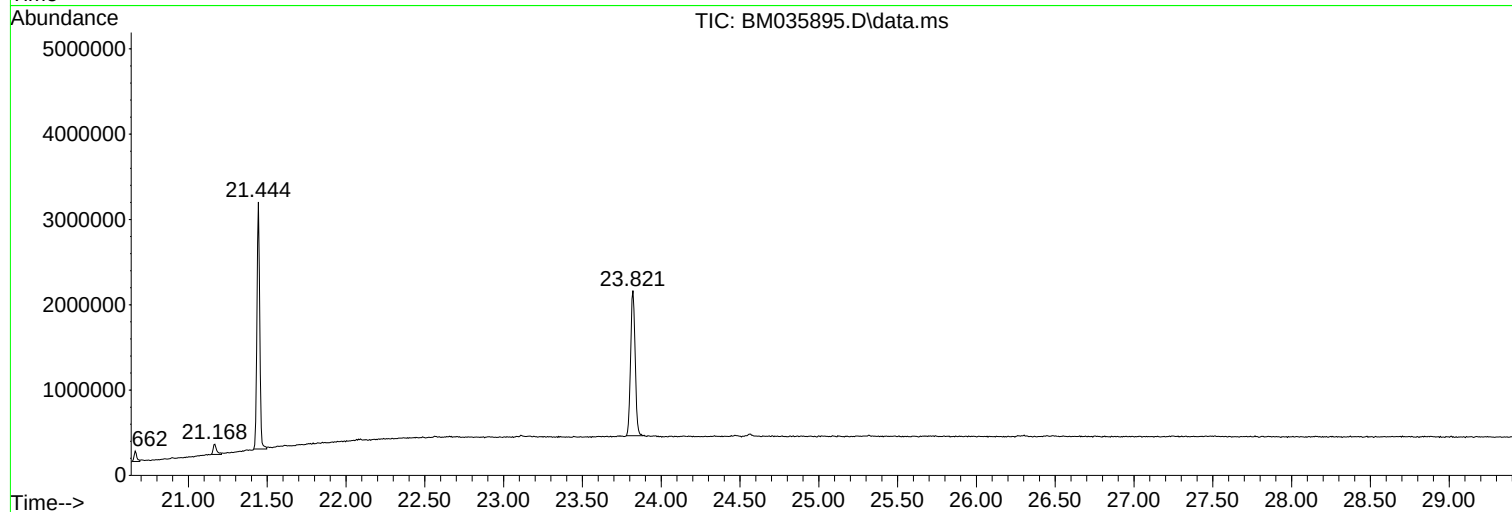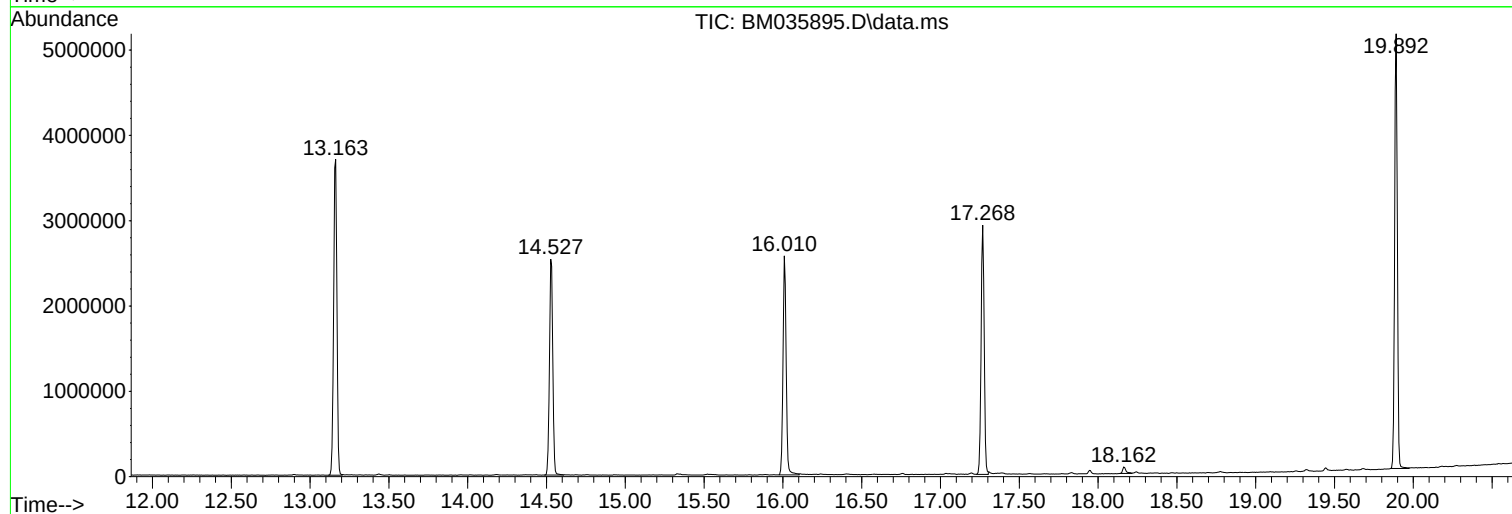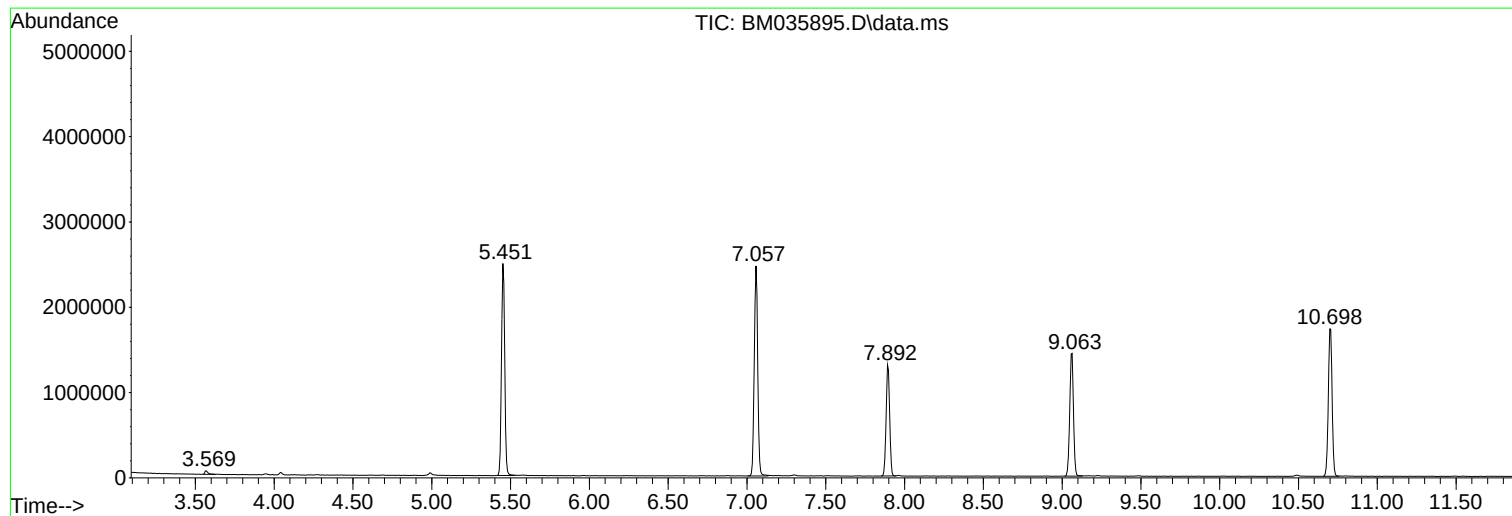

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035895.D
Acq On : 21 Jul 2022 18:55
Operator : CG/JU
Sample : N3786-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC17A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035895.D
Acq On : 21 Jul 2022 18:55
Operator : CG/JU
Sample : N3786-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC17A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------