

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035896.D
 Acq On : 21 Jul 2022 19:32
 Operator : CG/JU
 Sample : N3786-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0718-WC-TP-12EB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.569	78	82	89	rBV	87667	114407	1.38%	0.214%
2	4.993	318	324	335	rVB	109219	171150	2.07%	0.321%
3	5.457	396	403	418	rBV	4431139	6351967	76.68%	11.899%
4	7.057	667	675	692	rBV	4130266	6457733	77.96%	12.097%
5	7.893	810	817	824	rBV	1132831	1758529	21.23%	3.294%
6	9.063	1006	1016	1027	rBV	2474761	4001719	48.31%	7.496%
7	10.698	1284	1294	1303	rBV	1440012	2376337	28.69%	4.451%
8	13.163	1705	1713	1724	rBV	5769990	8283209	100.00%	15.516%
9	14.527	1937	1945	1954	rBV	1903047	2716414	32.79%	5.088%
10	16.010	2191	2197	2213	rBV	3517729	4868046	58.77%	9.119%
11	17.268	2404	2411	2421	rBV	1897825	2687867	32.45%	5.035%
12	17.945	2522	2526	2531	rBV	111247	136444	1.65%	0.256%
13	18.162	2559	2563	2572	rBV	115371	179112	2.16%	0.336%
14	19.121	2718	2726	2730	rBV	170365	205664	2.48%	0.385%
15	19.892	2851	2857	2868	rBV	6739284	7856144	94.84%	14.716%
16	20.662	2984	2988	2991	rBV	108888	129547	1.56%	0.243%
17	21.162	3069	3073	3085	rBV2	272826	444397	5.37%	0.832%
18	21.439	3116	3120	3132	rBV	1766369	2319998	28.01%	4.346%
19	23.815	3518	3524	3533	rBV2	1213325	2325725	28.08%	4.357%




Sum of corrected areas: 53384409

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035896.D
Acq On : 21 Jul 2022 19:32
Operator : CG/JU
Sample : N3786-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-12EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

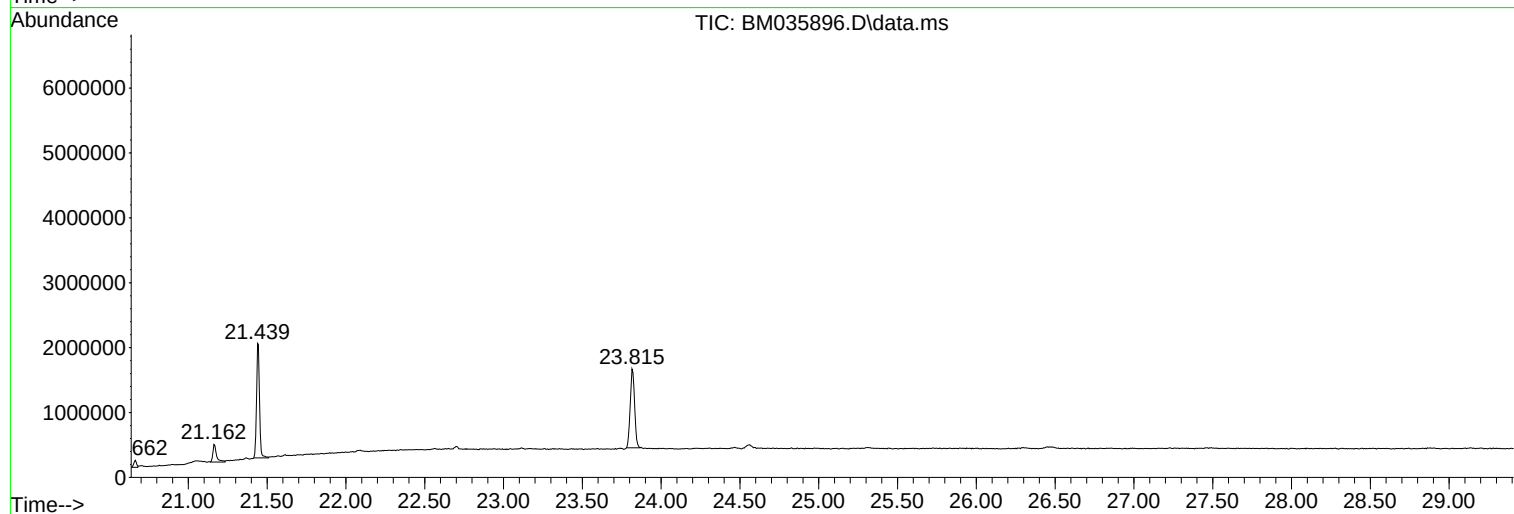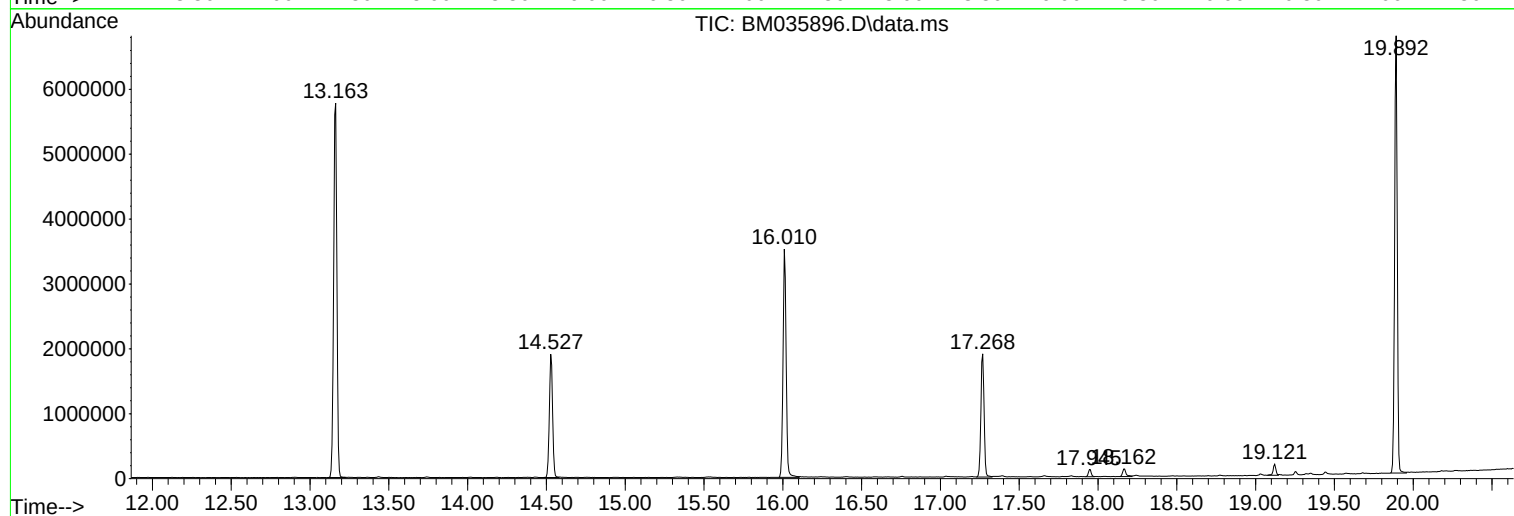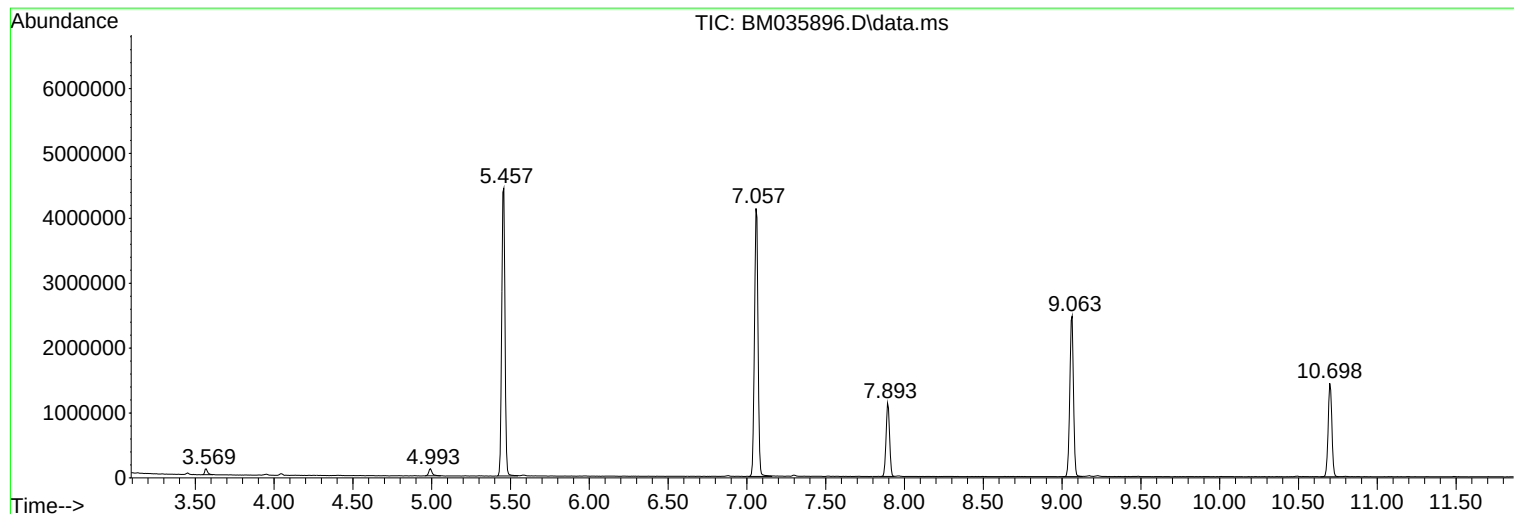

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035896.D
Acq On : 21 Jul 2022 19:32
Operator : CG/JU
Sample : N3786-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-12EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035896.D
Acq On : 21 Jul 2022 19:32
Operator : CG/JU
Sample : N3786-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-12EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------