

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035898.D
 Acq On : 21 Jul 2022 20:46
 Operator : CG/JU
 Sample : N3786-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0718-WC-TP-WC5B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	317	323	333	rBV	85133	130541	3.08%	0.358%
2	5.452	394	402	412	rBV	2177119	3075439	72.52%	8.438%
3	7.057	667	675	685	rBV	2102854	3155196	74.40%	8.657%
4	7.893	811	817	825	rBV	1199978	1855050	43.74%	5.090%
5	9.057	1008	1015	1025	rBV	1195580	1968478	46.41%	5.401%
6	10.698	1285	1294	1306	rBV	1544586	2575591	60.73%	7.067%
7	13.157	1705	1712	1723	rBV	2802640	4091650	96.48%	11.226%
8	14.527	1934	1945	1954	rBV	2049066	2909129	68.59%	7.982%
9	16.010	2190	2197	2213	rBV	1657196	2314788	54.58%	6.351%
10	17.268	2404	2411	2416	rBV	2141611	2970556	70.04%	8.150%
11	17.310	2416	2418	2424	rVB	65429	73280	1.73%	0.201%
12	18.162	2558	2563	2566	rBV3	56412	77820	1.83%	0.214%
13	19.321	2755	2760	2764	rBV	110378	147408	3.48%	0.404%
14	19.680	2817	2821	2830	rVB	107831	157676	3.72%	0.433%
15	19.886	2851	2856	2865	rBV	3465170	4241039	100.00%	11.636%
16	20.662	2984	2988	2993	rBV	106682	135540	3.20%	0.372%
17	21.162	3070	3073	3079	rBV5	127398	181797	4.29%	0.499%
18	21.439	3115	3120	3125	rBV2	2585483	3181846	75.03%	8.730%
19	23.815	3517	3524	3537	rVB2	1599612	3203893	75.55%	8.791%




Sum of corrected areas: 36446717

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035898.D
Acq On : 21 Jul 2022 20:46
Operator : CG/JU
Sample : N3786-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC5B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

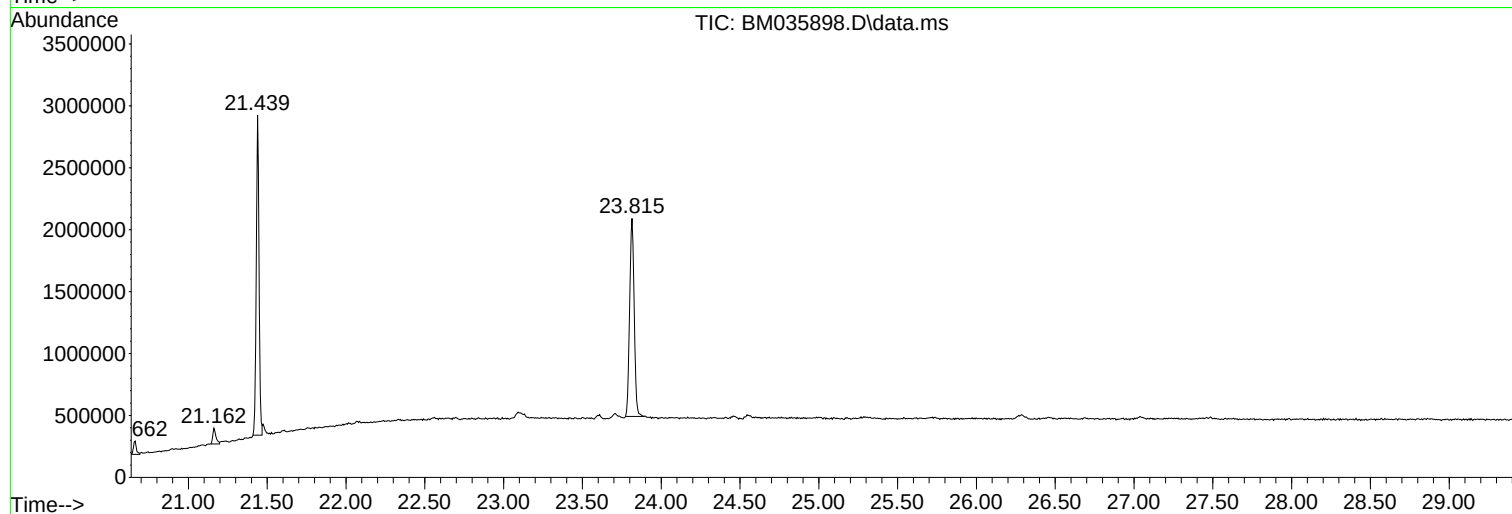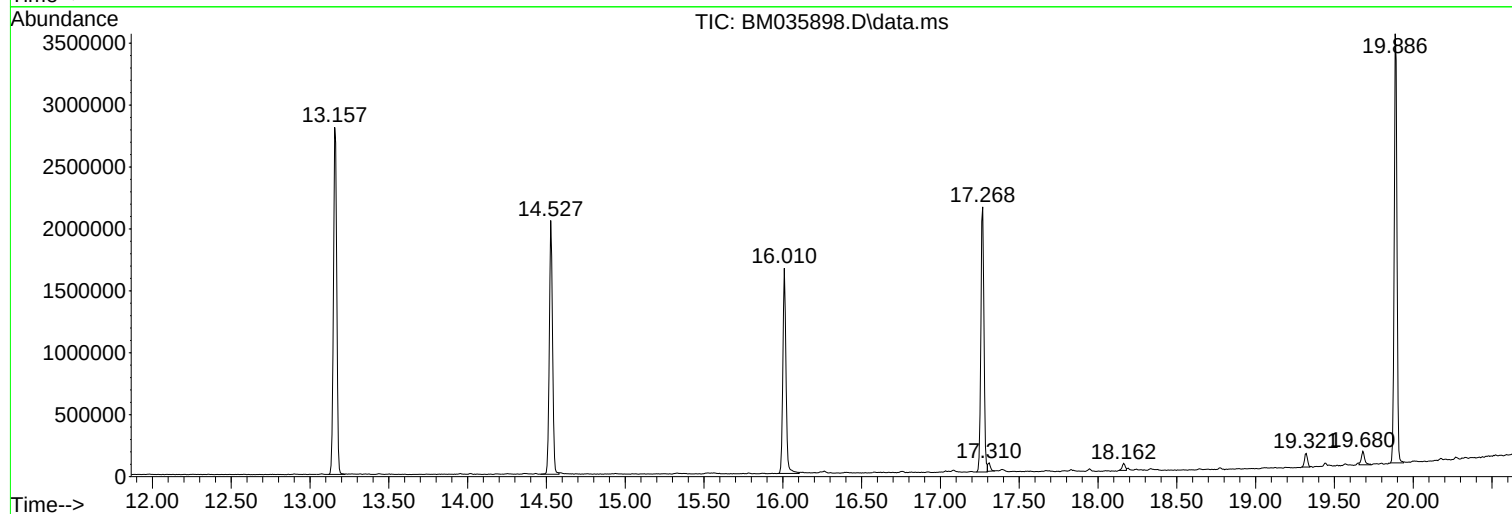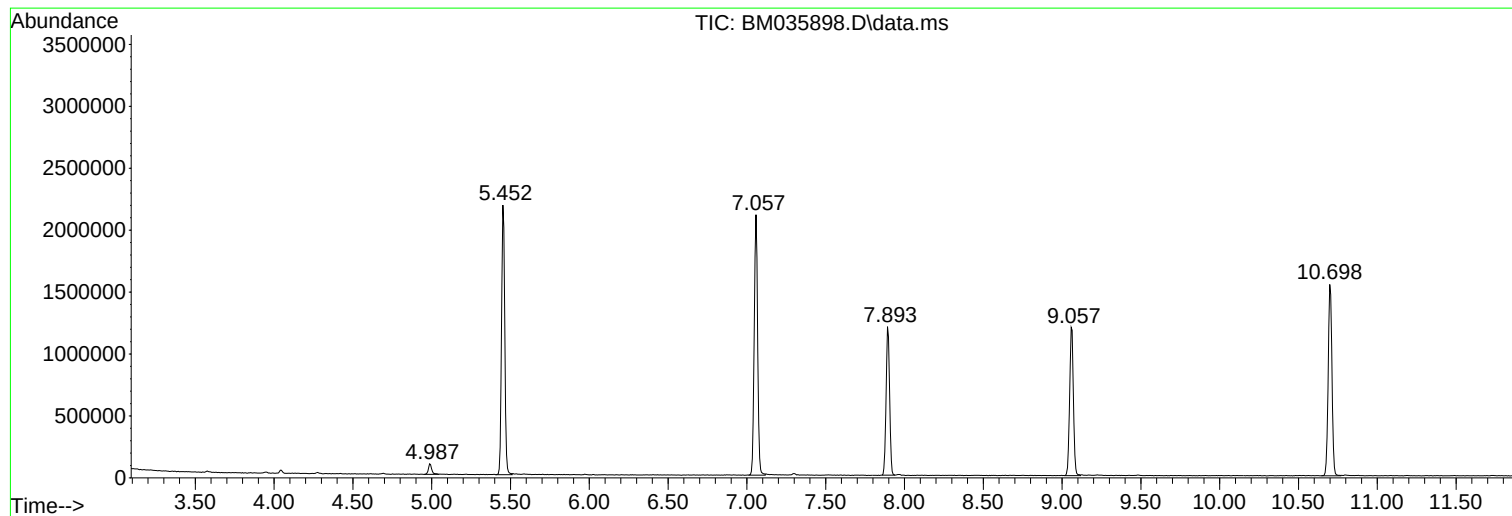

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035898.D
Acq On : 21 Jul 2022 20:46
Operator : CG/JU
Sample : N3786-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC5B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035898.D
Acq On : 21 Jul 2022 20:46
Operator : CG/JU
Sample : N3786-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC5B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------