

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035899.D
 Acq On : 21 Jul 2022 21:24
 Operator : CG/JU
 Sample : N3786-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0718-WC-TP-WC3EA

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	318	323	333	rBV	49084	77077	1.92%	0.211%
2	5.451	396	402	414	rBV	1868231	2603022	64.88%	7.127%
3	7.057	666	675	687	rBV	1805919	2785976	69.44%	7.628%
4	7.892	809	817	825	rBV	1332066	2013535	50.19%	5.513%
5	9.057	1007	1015	1026	rBV	1072004	1725361	43.01%	4.724%
6	10.698	1286	1294	1306	rBV	1790852	2939959	73.28%	8.050%
7	13.157	1705	1712	1725	rBV	2754946	3887036	96.89%	10.643%
8	13.433	1753	1759	1767	rBV	33957	58711	1.46%	0.161%
9	14.527	1938	1945	1960	rBV	2483874	3555700	88.63%	9.735%
10	16.009	2191	2197	2212	rBV	1603879	2252481	56.14%	6.167%
11	17.268	2404	2411	2421	rBV	2649066	3659198	91.21%	10.019%
12	17.945	2521	2526	2532	rBV	39846	51814	1.29%	0.142%
13	18.162	2559	2563	2569	rBV3	50685	65594	1.63%	0.180%
14	19.886	2851	2856	2865	rBV	3169248	4011972	100.00%	10.985%
15	20.662	2985	2988	2991	rBV	97692	105701	2.63%	0.289%
16	21.162	3069	3073	3080	rBV	173985	281019	7.00%	0.769%
17	21.439	3115	3120	3129	rBV	2606978	3291321	82.04%	9.012%
18	23.815	3517	3524	3534	rBV2	1578331	3157925	78.71%	8.646%




Sum of corrected areas: 36523402

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035899.D
Acq On : 21 Jul 2022 21:24
Operator : CG/JU
Sample : N3786-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC3EA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

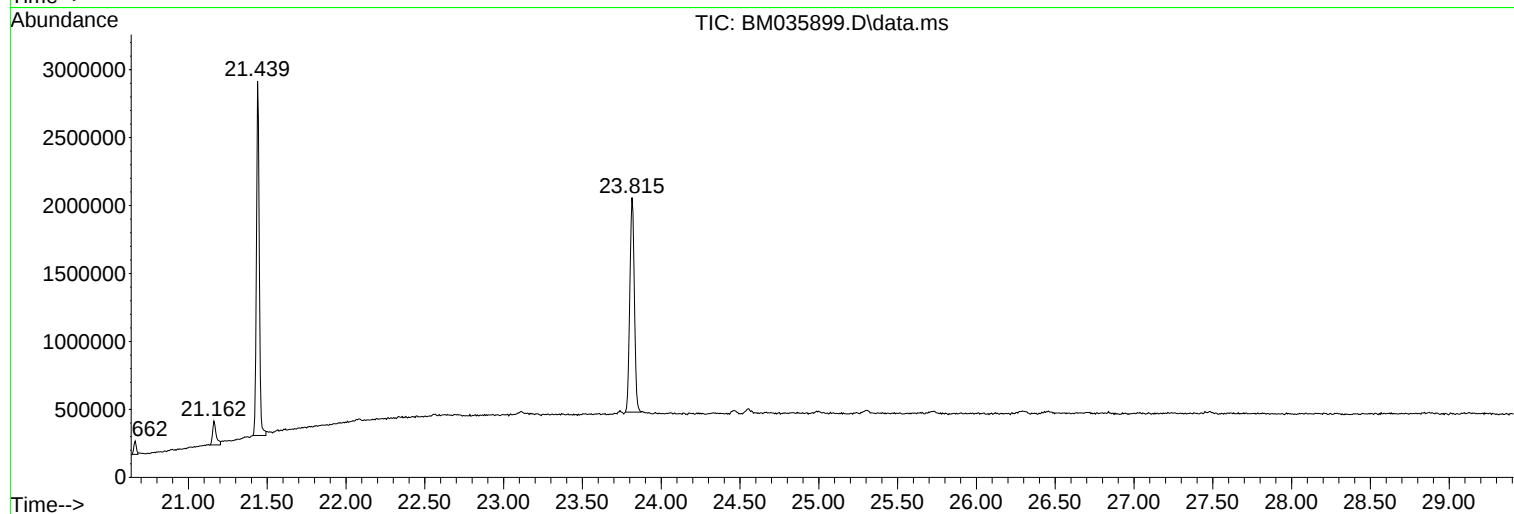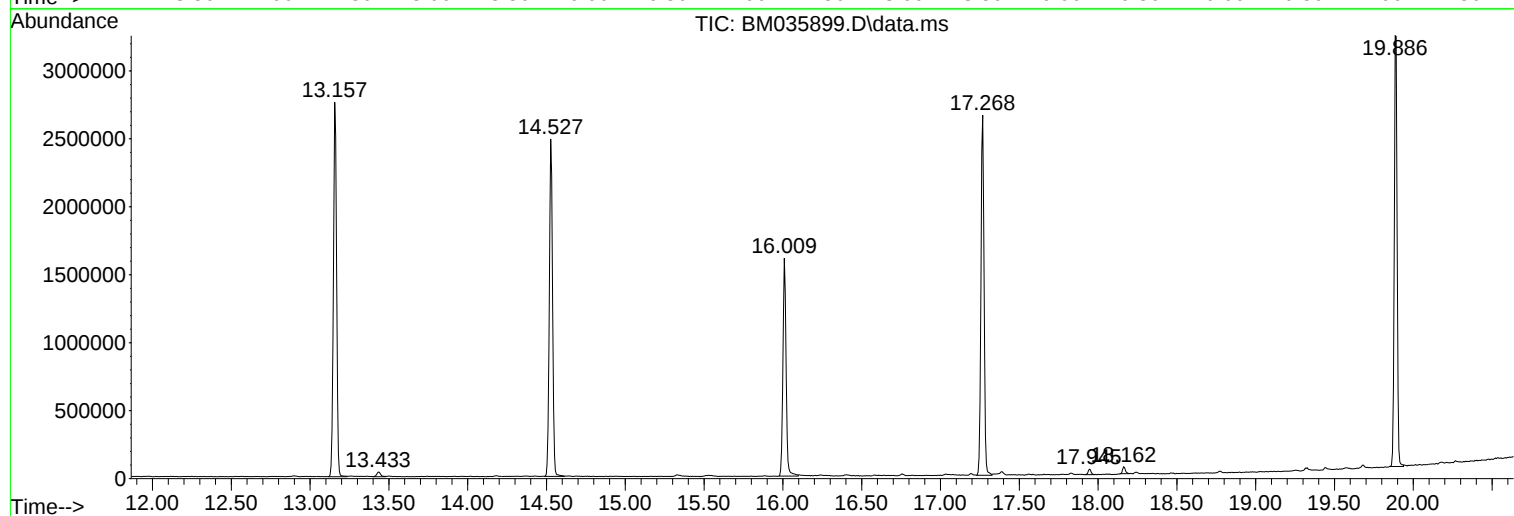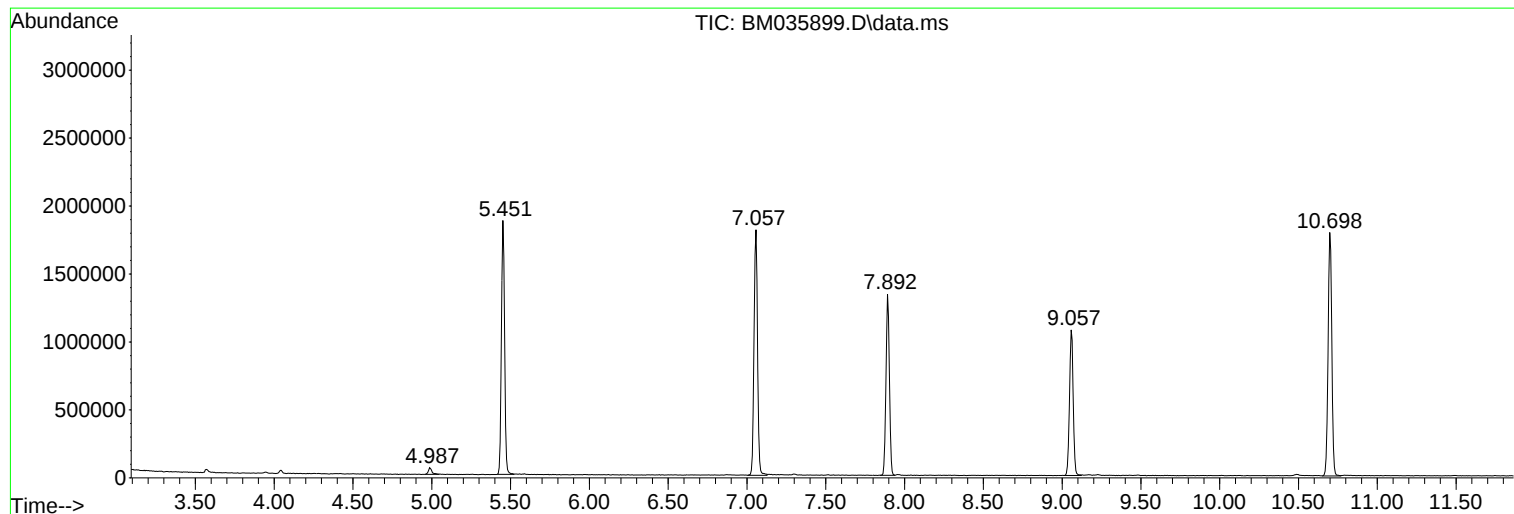

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035899.D
Acq On : 21 Jul 2022 21:24
Operator : CG/JU
Sample : N3786-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC3EA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035899.D
Acq On : 21 Jul 2022 21:24
Operator : CG/JU
Sample : N3786-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC3EA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------