
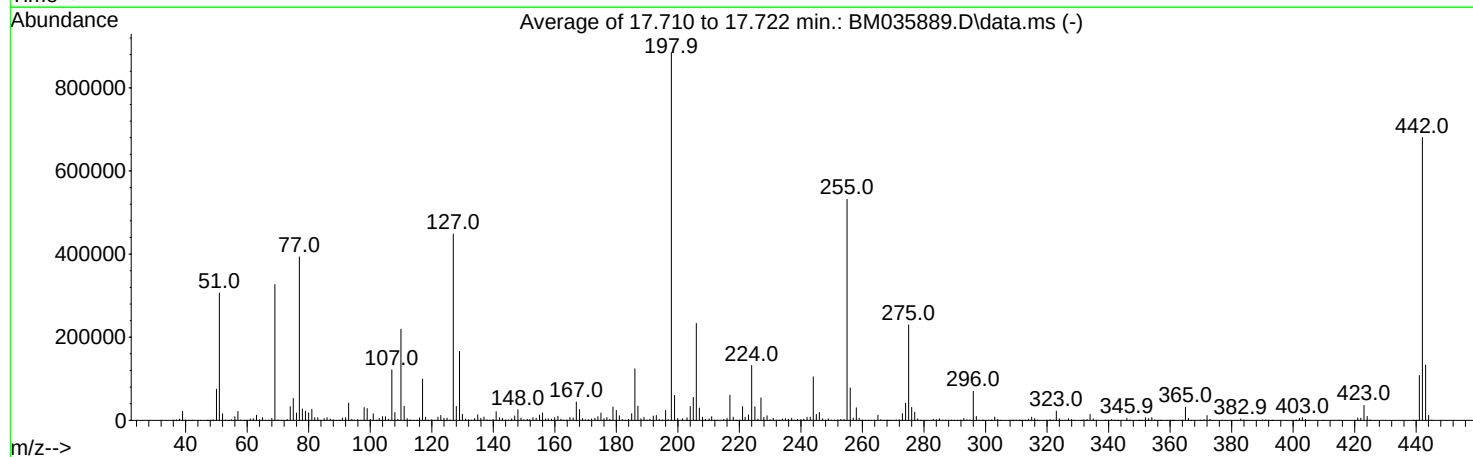


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035889.D
 Acq On : 21 Jul 2022 14:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 22 14:25:12 2022

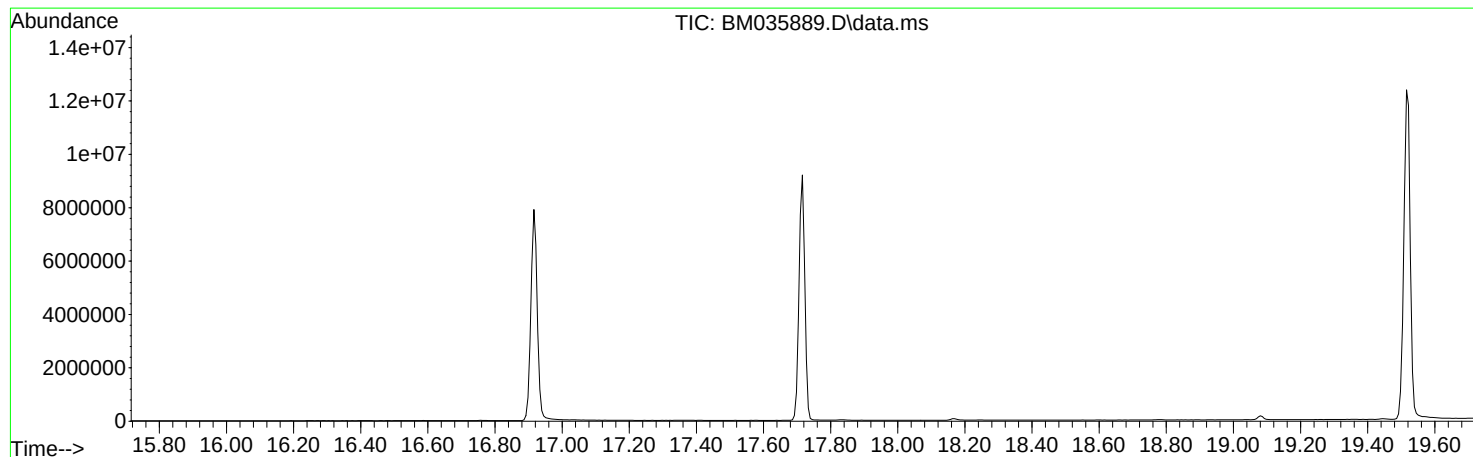




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	306104	PASS
68	69	0.00	2	1.5	4789	PASS
69	198	0.00	100	36.9	326820	PASS
70	69	0.00	2	0.4	1352	PASS
127	198	10	80	50.7	448576	PASS
197	198	0.00	2	0.2	1933	PASS
198	198	100	100	100.0	884971	PASS
199	198	5	9	6.8	60101	PASS
275	198	10	60	26.0	229973	PASS
365	198	1	100	3.6	31667	PASS
441	198	0.01	100	12.2	107765	PASS
442	442	50	100	100.0	680555	PASS
443	442	15	24	19.6	133280	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
 Data File : BM035889.D
 Acq On : 21 Jul 2022 14:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 05:45:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 18 17:08:15 2022
 Response via : Initial Calibration

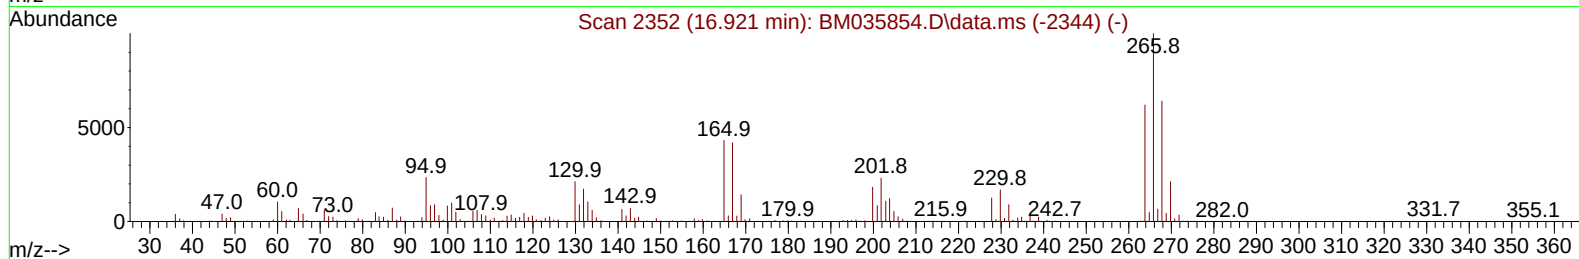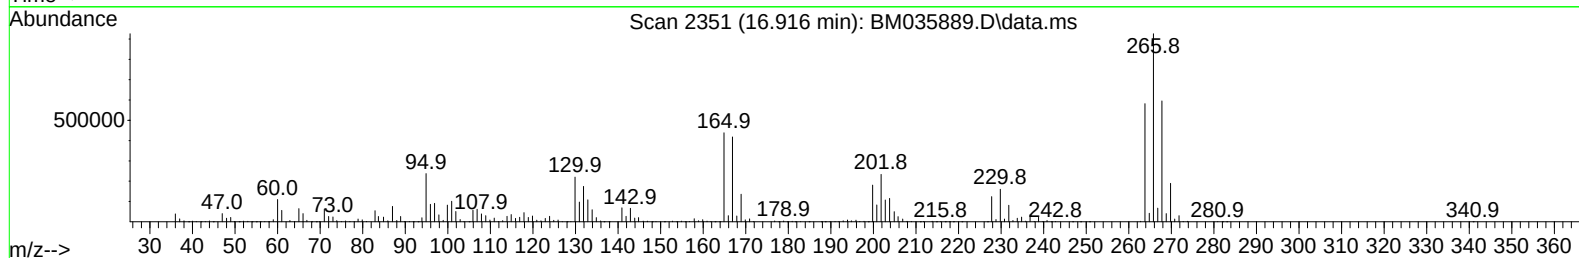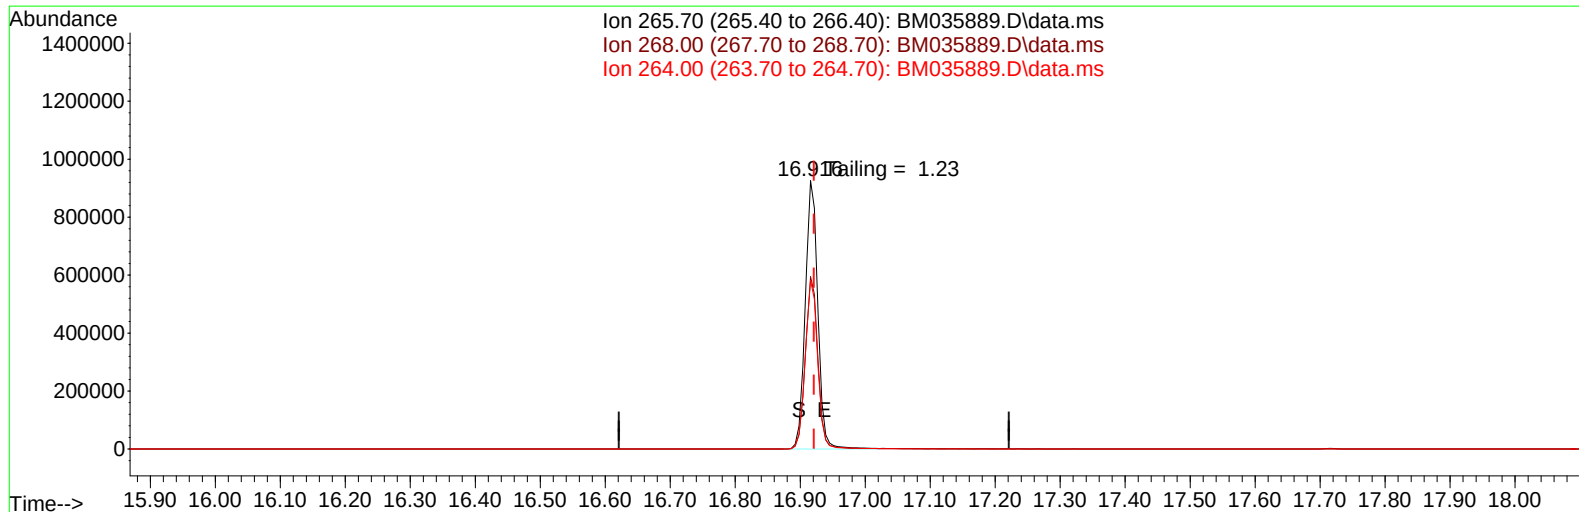

TIC: BM035889.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.005) 561785.15 ng




response 1251412

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.23
264.00	63.30	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072122\
Data File : BM035889.D
Acq On : 21 Jul 2022 14:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 22 05:45:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 18 17:08:15 2022
Response via : Initial Calibration

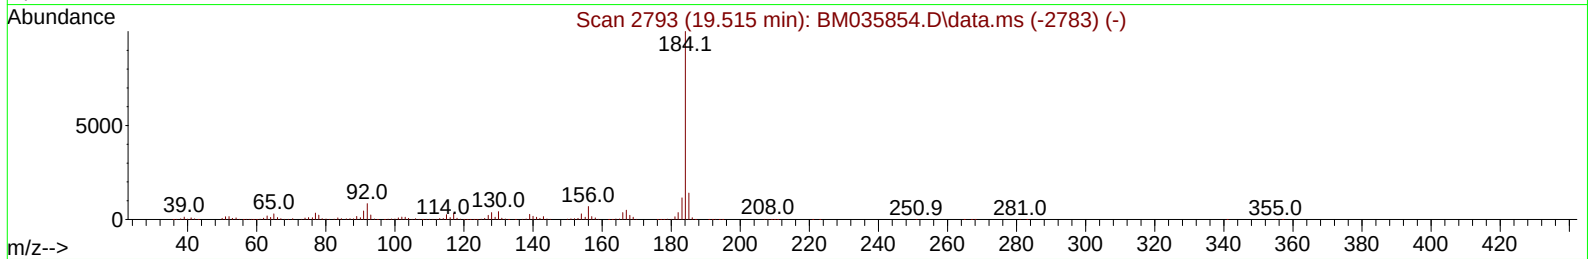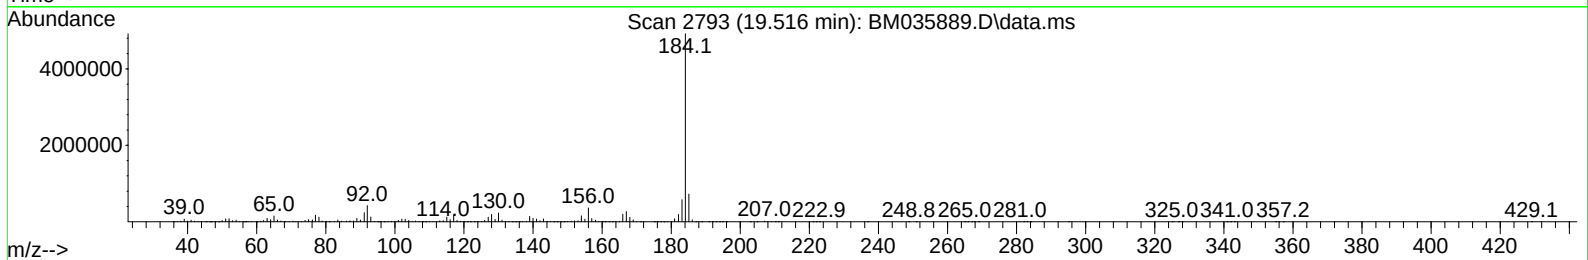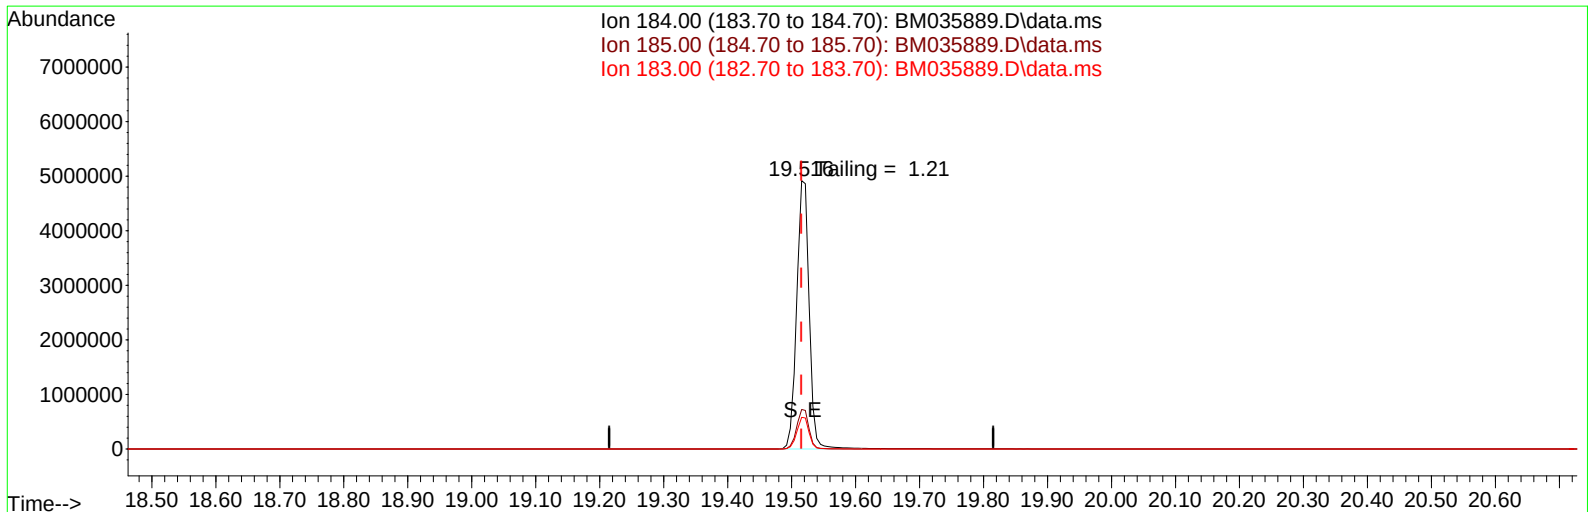

TIC: BM035889.D\data.ms

(77) Benzidine

19.516min (+ 0.001) 418848.34 ng

response 6721326

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.76
183.00	11.90	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/21/2022	BNA_M	<u>BM035889.D</u>
Compound Name	Response	Retention Time
DDT	3148523	20.751
DDD	24677	20.31
DDE	1142	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25819	3174342	0.81

Instrument :
BNA_M
ClientSampleId :
DFTPP