

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072216\
 Data File : BM006642.D
 Acq On : 23 Jul 2016 02:09
 Operator : UM/SJ
 Sample : H4076-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 D9YP3

Manual Integration

Quant Time: Jul 23 03:27:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 23 00:16:38 2016
 Response via : Initial Calibration

APPROVED
 sohil
 7/25/2016 6:39:28 PM

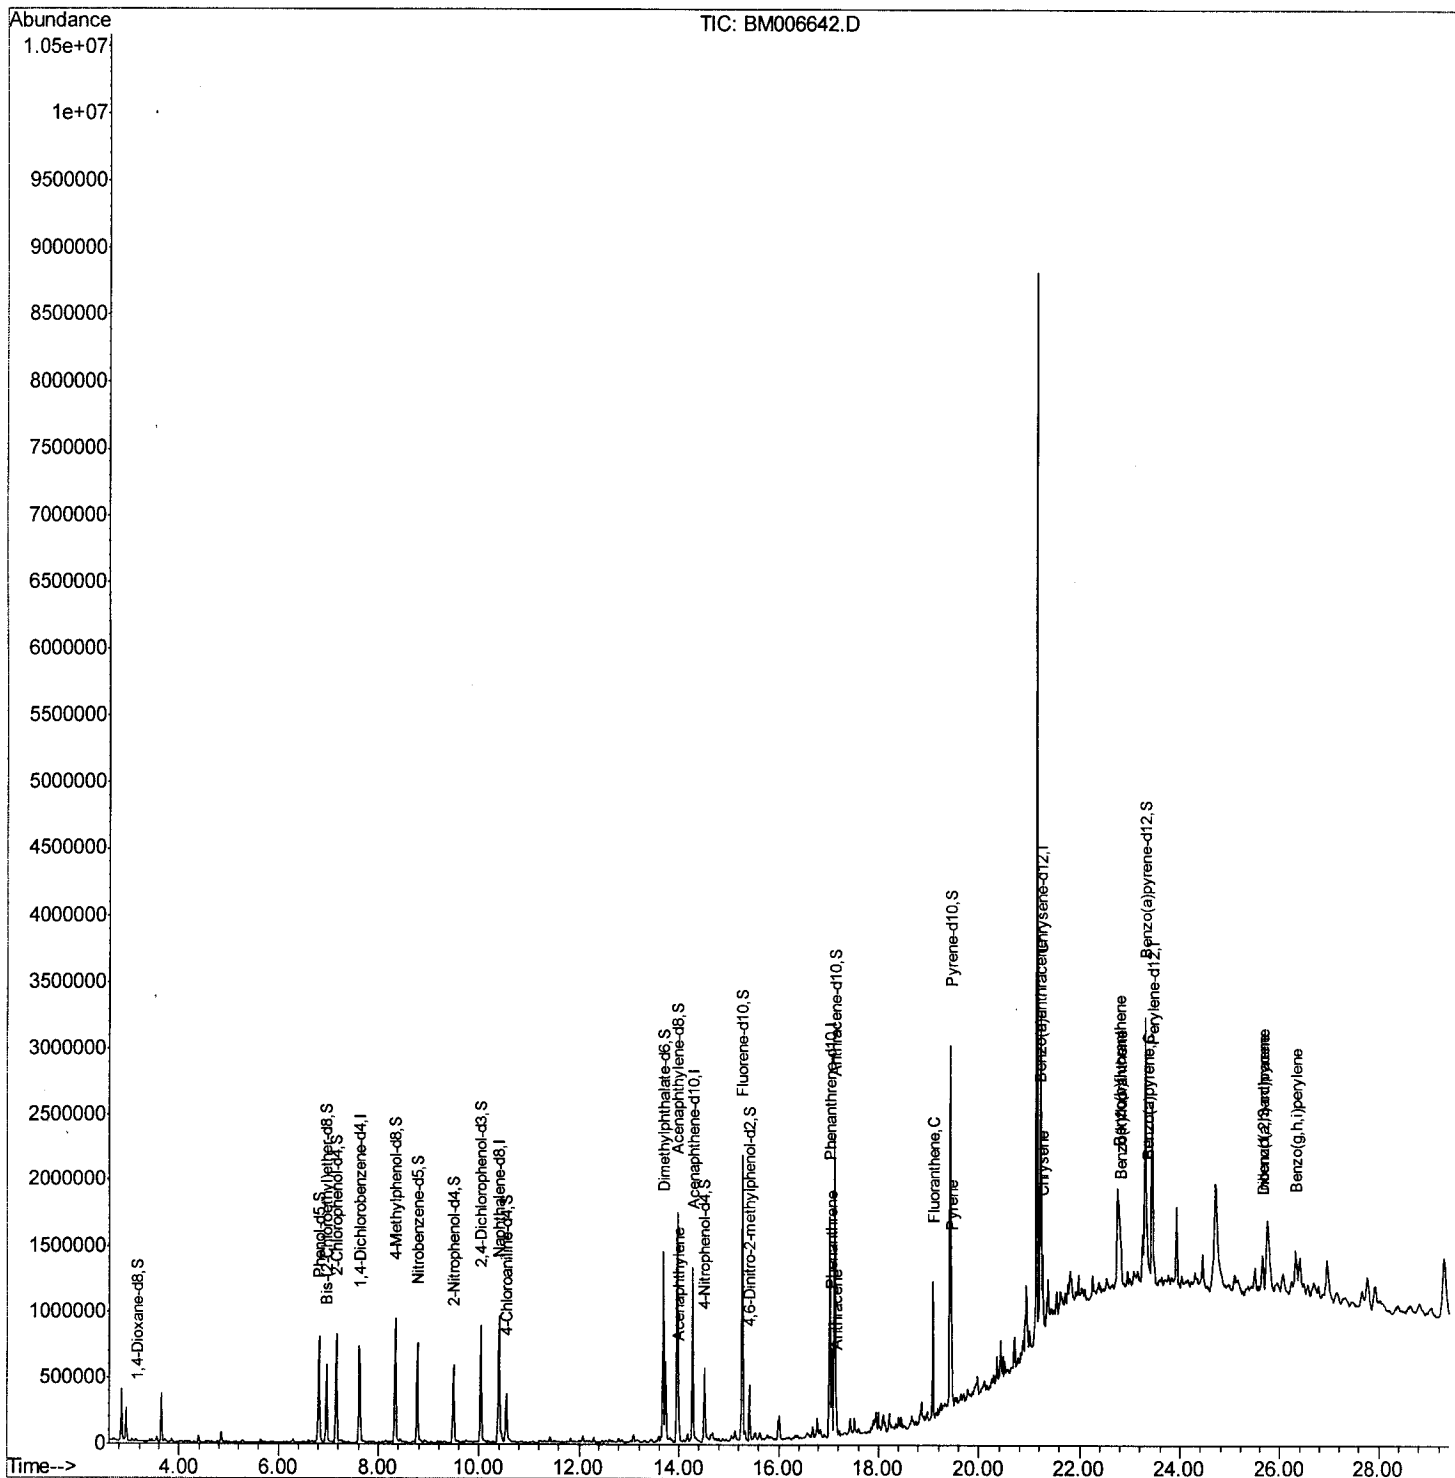

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072216\
 Data File : BM006642.D
 Acq On : 23 Jul 2016 02:09
 Operator : UM/SJ
 Sample : H4076-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 D9YP3

Manual Integration

APPROVED
 sohil
 7/25/2016 6:39:28 PM

Quant Time: Jul 23 03:13:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 23 00:16:38 2016
 Response via : Initial Calibration

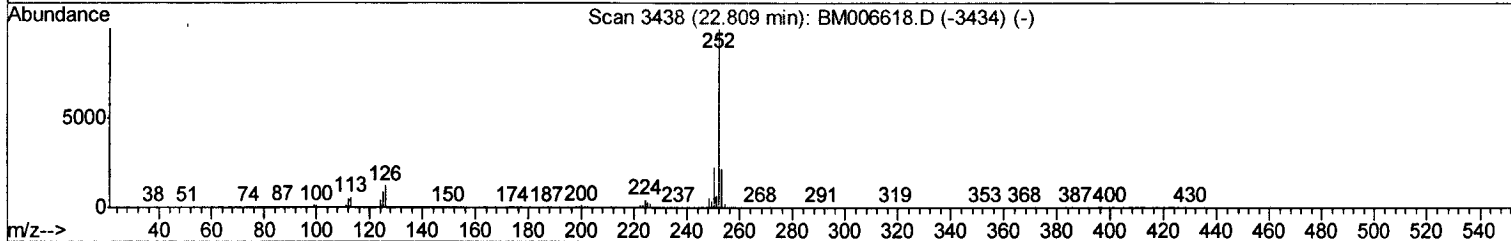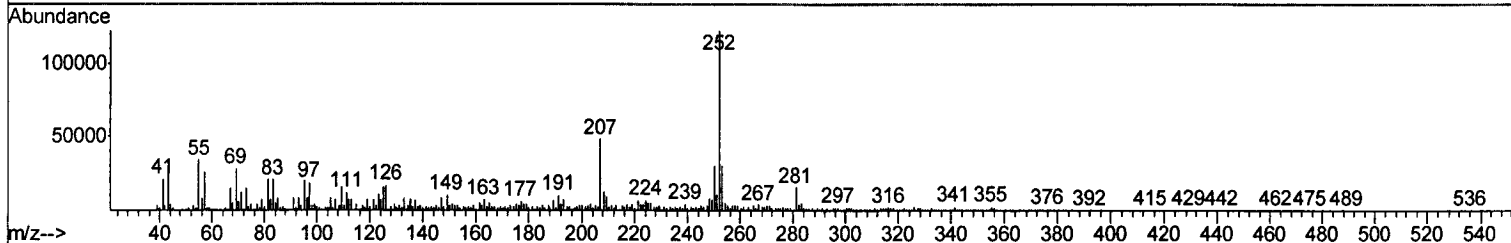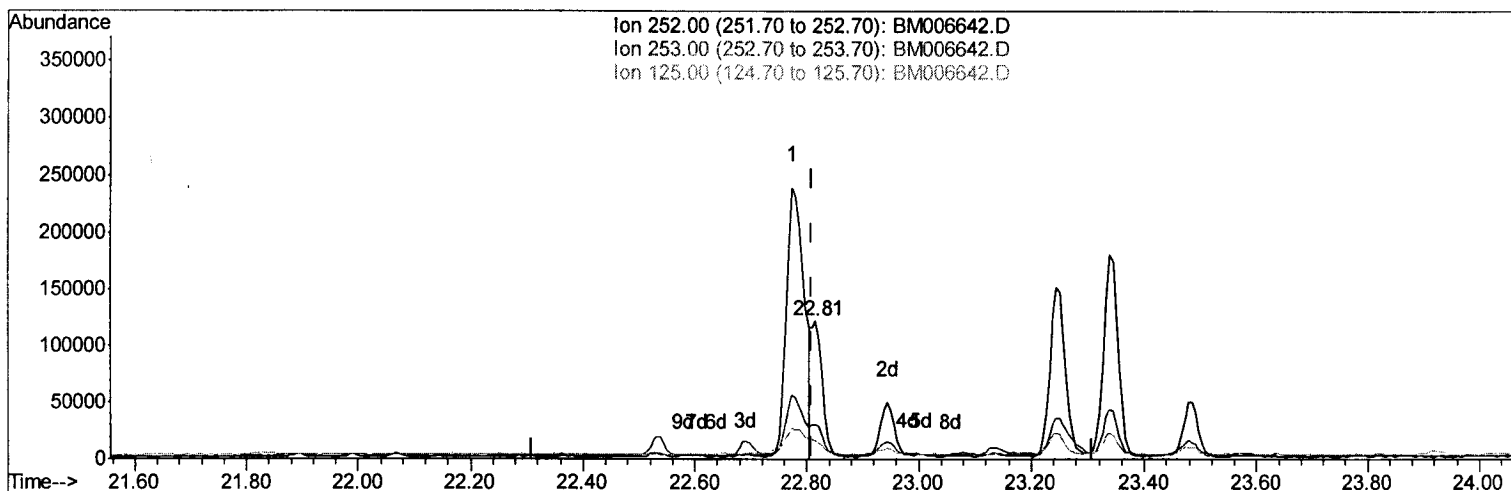

TIC: BM006642.D

(36) Benzo(k)fluoranthene

22.815min (+0.006) 2.81ng/ul m *V.M*
07/26/16
 response 175251

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	24.62
125.00	9.60	13.34#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072216\
 Data File : BM006642.D
 Acq On : 23 Jul 2016 02:09
 Operator : UM/SJ
 Sample : H4076-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 D9YP3

Quant Time: Jul 23 03:13:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 23 00:16:38 2016
 Response via : Initial Calibration

Manual Integration
 APPROVED
 sohil
 7/25/2016 6:39:28 PM

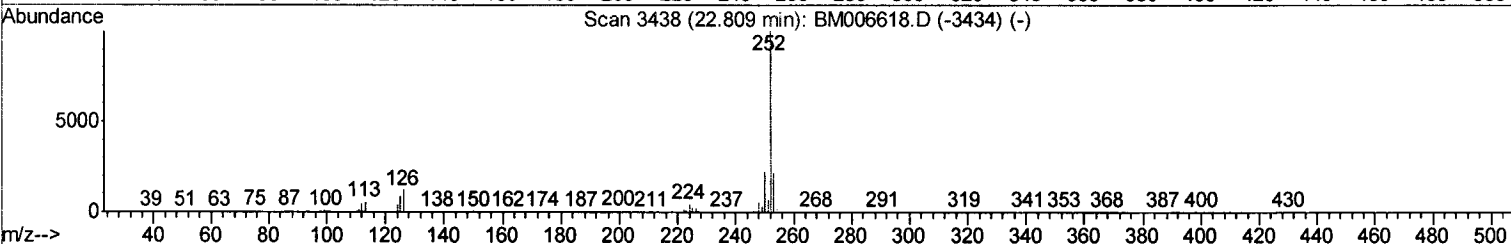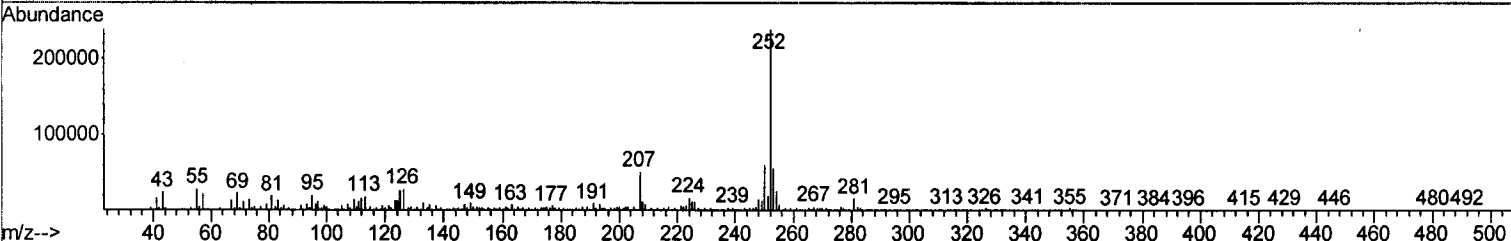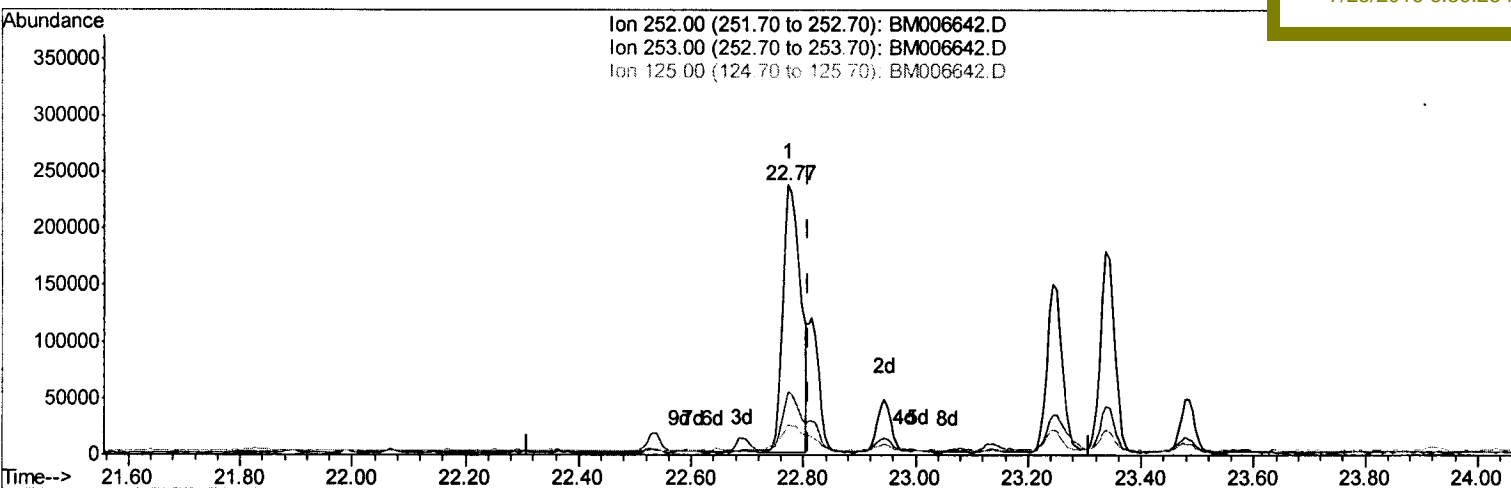

(36) Benzo(k)fluoranthene
 22.774min (-0.035) 8.21ng/ul
 response 512318

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.51
125.00	9.60	11.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072216\
 Data File : BM006642.D
 Acq On : 23 Jul 2016 02:09
 Operator : UM/SJ
 Sample : H4076-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YP3

Quant Time: Jul 23 03:27:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 23 00:16:38 2016
 Response via : Initial Calibration

Manual Integration
 APPROVED
 sohil
 7/25/2016 6:39:28 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	189462	20.00	ng/ul	0.01
7) Naphthalene-d8	10.40	136	795332	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.27	164	436398	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.03	188	985297	20.00	ng/ul	0.01
29) Chrysene-d12	21.23	240	1030596	20.00	ng/ul	0.00
34) Perylene-d12	23.44	264	1076999	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.14	96	11667	2.49	ng/uL	0.00
3) Phenol-d5	6.81	99	449410	27.88	ng/ul	0.01
4) Bis-(2-Chloroethyl) ether-d	6.96	67	272649	27.31	ng/ul	0.00
5) 2-Chlorophenol-d4	7.16	132	356871	27.71	ng/ul	0.00
6) 4-Methylphenol-d8	8.33	113	350754	28.06	ng/ul	0.00
8) Nitrobenzene-d5	8.77	128	170482	28.32	ng/ul	0.00
9) 2-Nitrophenol-d4	9.49	143	181203	28.30	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.03	165	332860	27.51	ng/ul	0.01
12) 4-Chloroaniline-d4	10.55	131	220847	16.58	ng/ul	0.01
16) Dimethylphthalate-d6	13.69	166	941811	27.53	ng/ul	0.00
17) Acenaphthylene-d8	13.96	160	1245898	28.53	ng/ul	0.00
20) 4-Nitrophenol-d4	14.51	143	142371	23.96	ng/ul	0.02
21) Fluorene-d10	15.27	176	855731	27.96	ng/ul	0.01
24) 4,6-Dinitro-2-methylphenol	15.42	200	79188	15.48	ng/ul	0.01
26) Anthracene-d10	17.13	188	1310412	28.01	ng/ul	0.01
30) Pyrene-d10	19.43	212	1422136	30.28	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.30	264	1383185	27.92	ng/ul	0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
18) Acenaphthylene	13.99	152	66000	1.41	ng/ul	98
25) Phenanthrene	17.07	178	388287	7.01	ng/ul	100
27) Anthracene	17.16	178	101005	1.77	ng/ul	99
28) Fluoranthene	19.09	202	614625	9.44	ng/ul	99
31) Pyrene	19.46	202	506308	8.11	ng/ul	96
32) Benzo(a)anthracene	21.21	228	315965	5.06	ng/ul	97
33) Chrysene	21.26	228	334605	5.81	ng/ul	97
35) Benzo(b)fluoranthene	22.77	252	512318	7.94	ng/ul#	97
36) Benzo(k)fluoranthene	22.81	252	175251m	2.81	ng/ul	97
38) Benzo(a)pyrene	23.34	252	316533	5.04	ng/ul#	95
39) Indeno(1,2,3-cd)pyrene	25.65	276	275196	3.78	ng/ul	97
40) Dibenzo(a,h)anthracene	25.65	278	79735	1.32	ng/ul#	80
41) Benzo(g,h,i)perylene	26.33	276	257954	4.14	ng/ul	96

U.M
 07/26/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed