
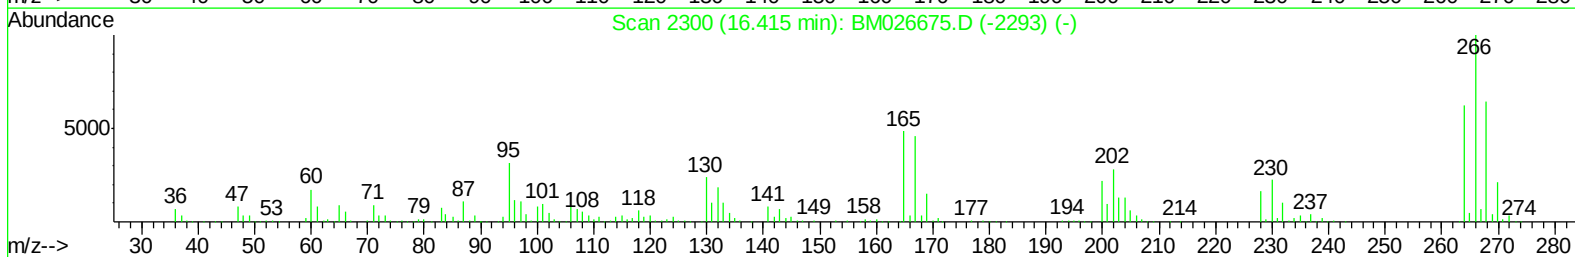
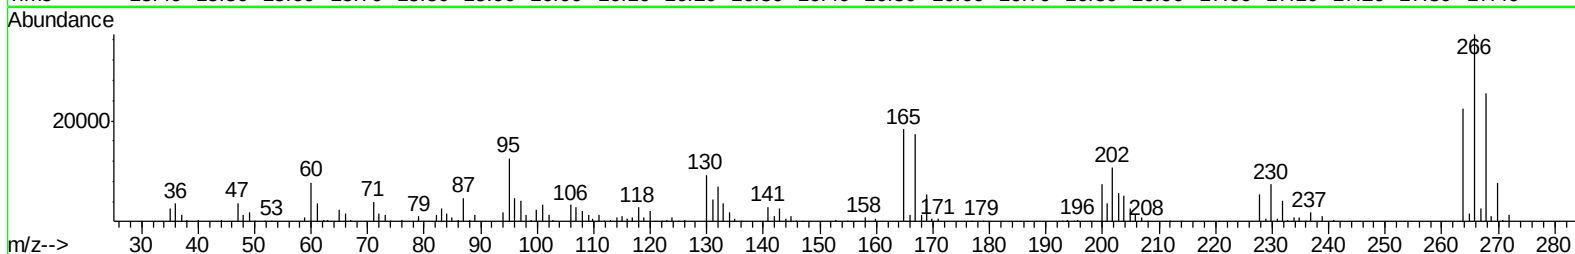


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072220\
Data File : BM026829.D
Acq On : 22 Jul 2020 12:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 03:27:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 22 14:16:10 2020
Response via : Initial Calibration

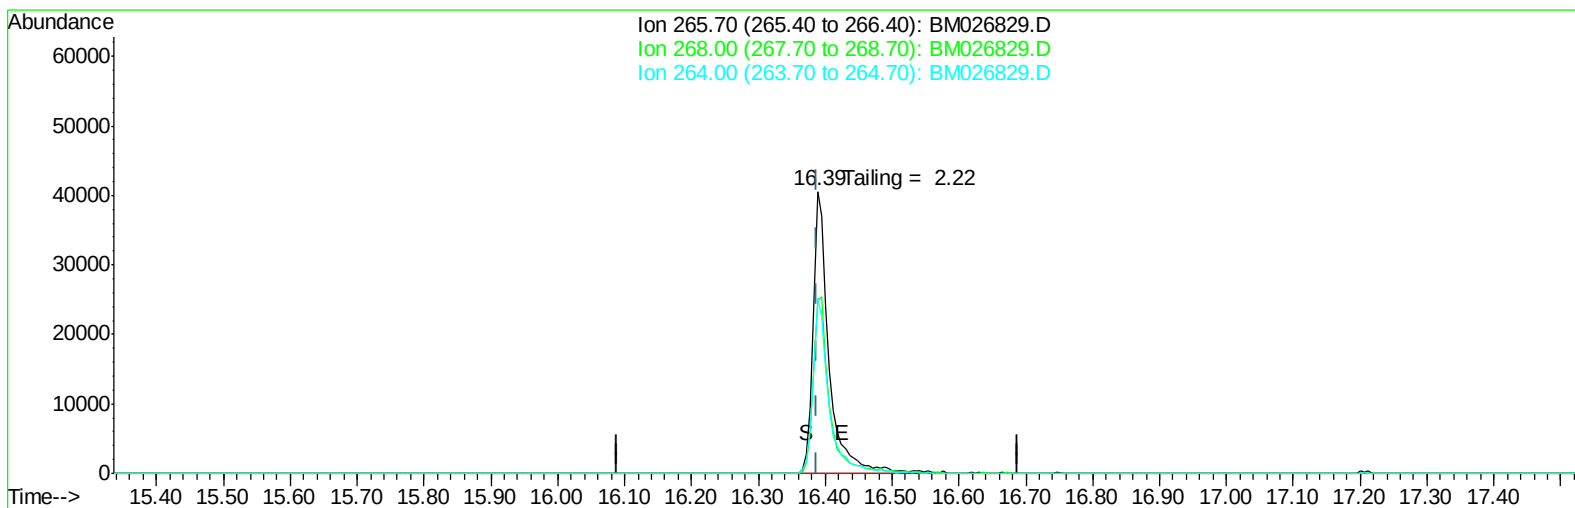

TIC: BM026829.D

(70) Pentachlorophenol (C)




16.389min (+0.000) 0.00ng

response 68345

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	61.45
264.00	62.60	62.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072220\
 Data File : BM026829.D
 Acq On : 22 Jul 2020 12:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 03:27:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 22 14:16:10 2020
 Response via : Initial Calibration

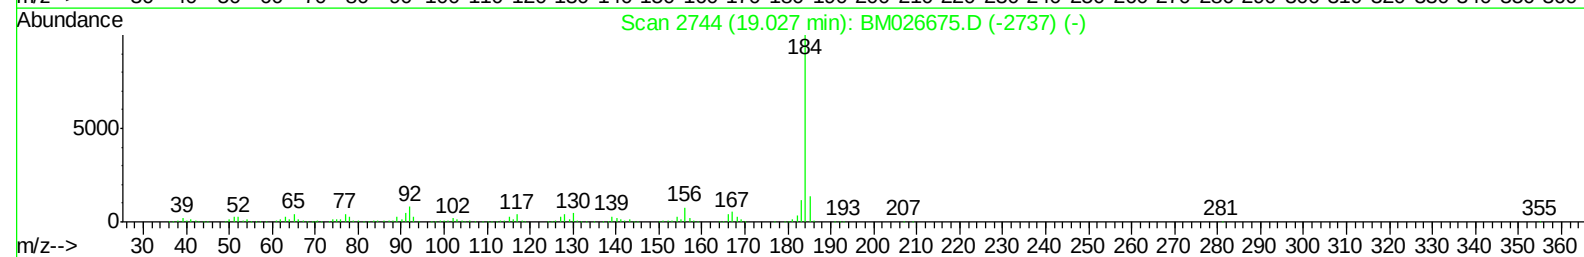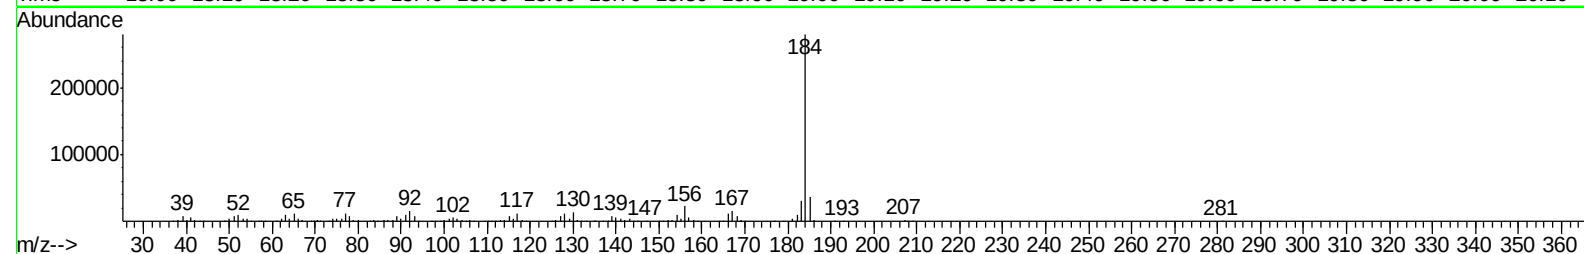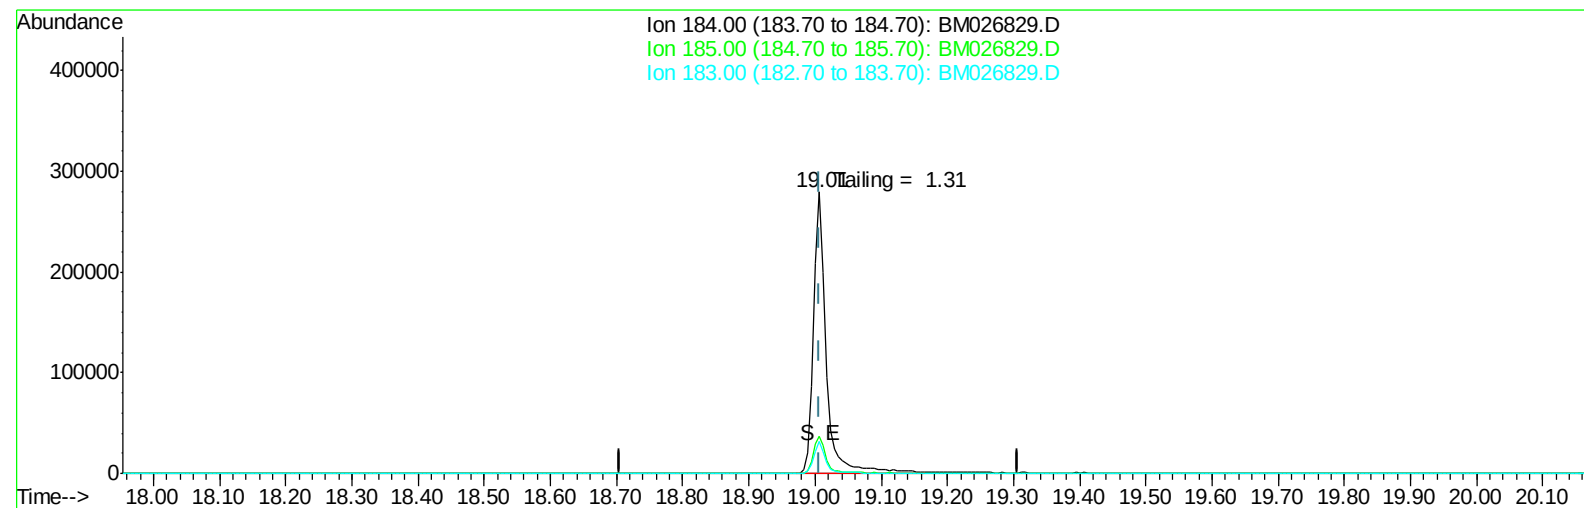

TIC: BM026829.D

(77) Benzidine

19.006min (+0.000) 0.00ng

response 379722

Ion	Exp%	Act%
184.00	100	100
185.00	13.60	13.16
183.00	11.60	11.21
0.00	0.00	0.00