


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072220\  
 Data File : BM026829.D  
 Acq On : 22 Jul 2020 12:57  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM070820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jul 22 14:16:10 2020

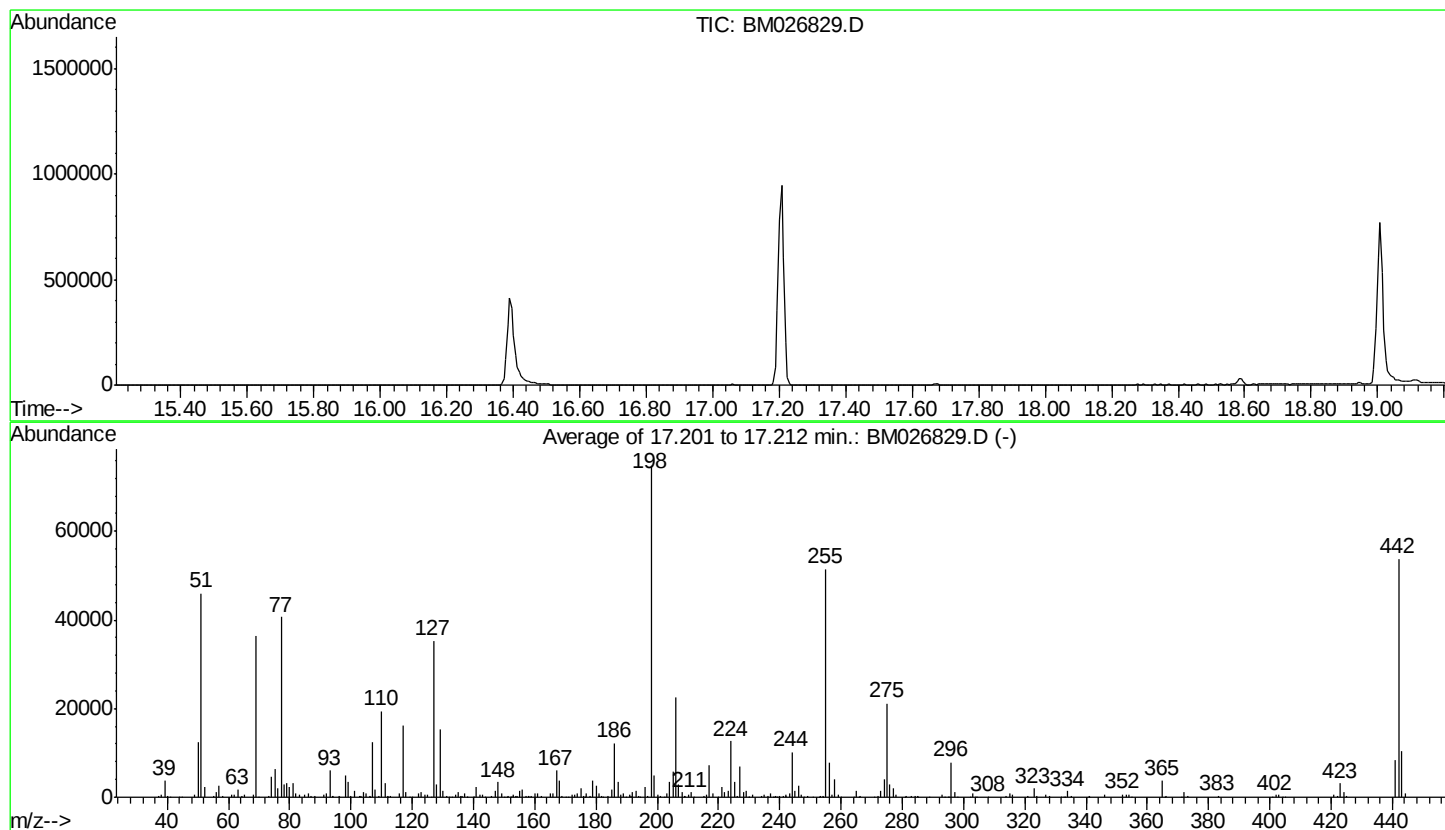

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 61.5      | 46021   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 657     | PASS             |
| 69          | 198          | 0.00         | 100          | 48.8      | 36496   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 106     | PASS             |
| 127         | 198          | 10           | 80           | 47.1      | 35258   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 442     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 74800   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 4946    | PASS             |
| 275         | 198          | 10           | 60           | 28.2      | 21088   | PASS             |
| 365         | 198          | 1            | 100          | 4.9       | 3679    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.3      | 8488    | PASS             |
| 442         | 198          | 50           | 100          | 71.9      | 53762   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 10320   | PASS             |